

AMBULATORY MEDICAL APPARATUS WITH
HAND HELD COMMUNICATION DEVICE

Attorney: Ted Rittmaster - 047711-0221

Foley & Lardner - 310-277-2223

Sheet 1 of 16

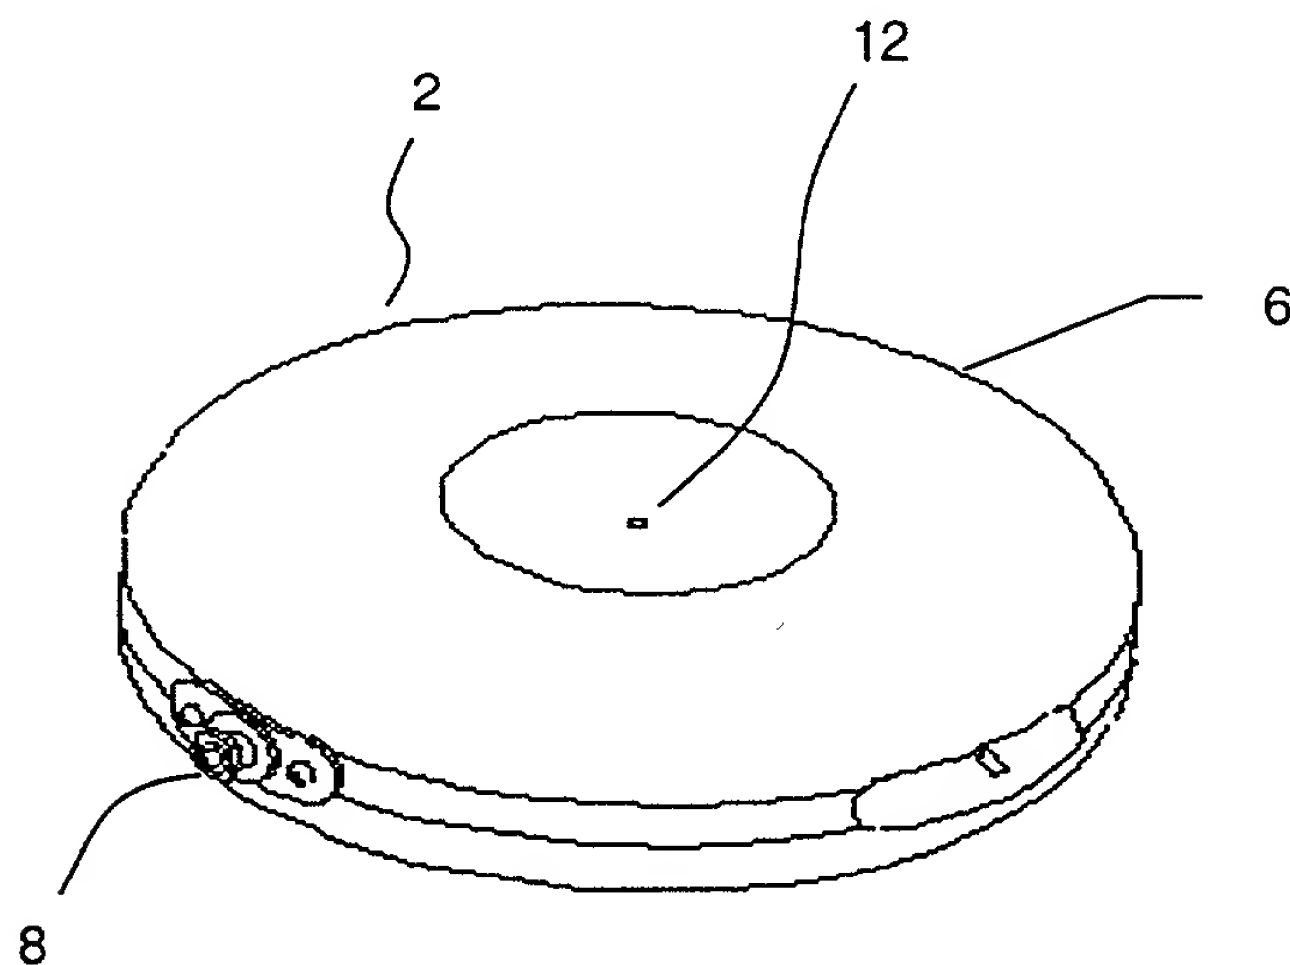


FIGURE 1A

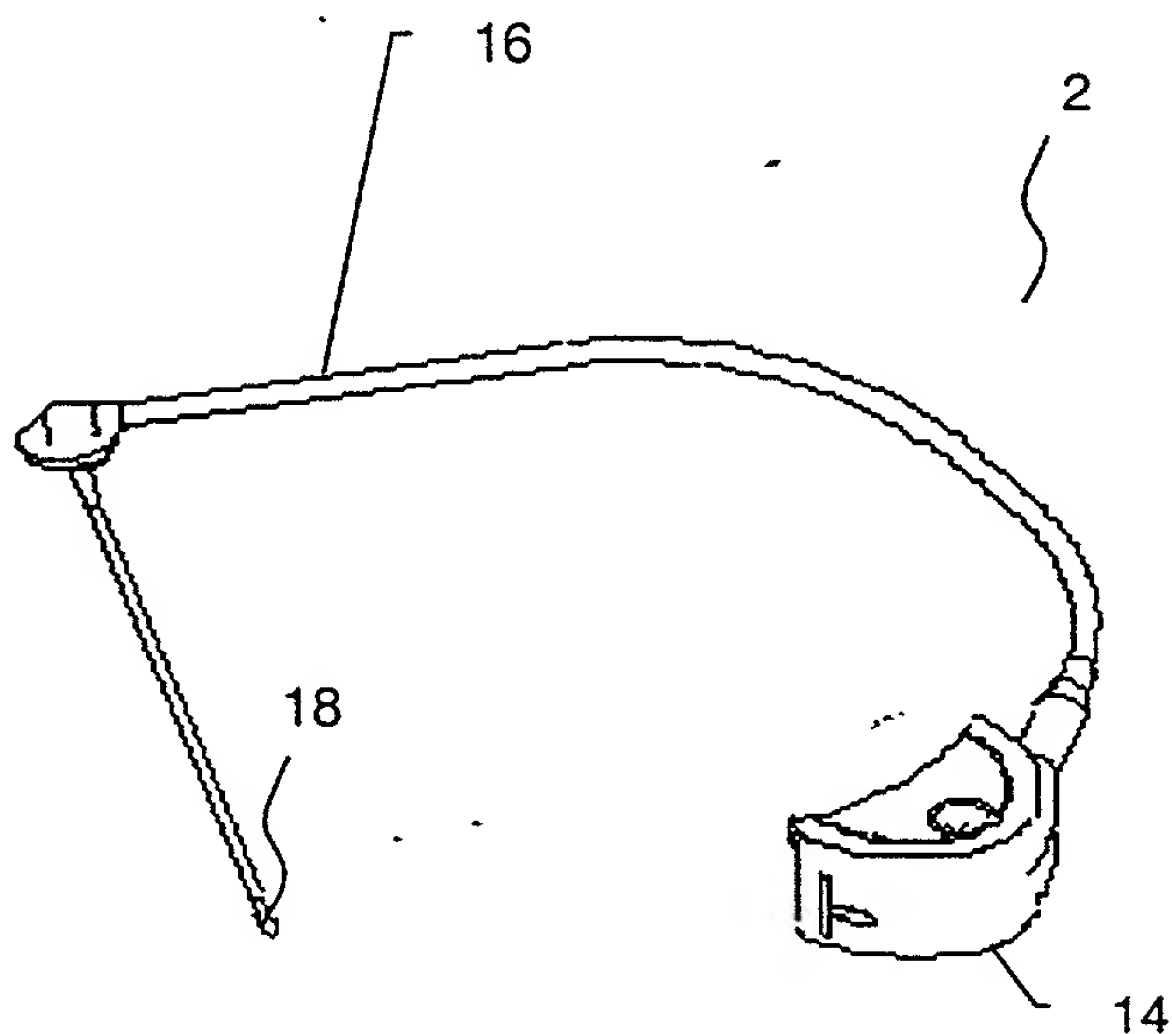


FIGURE 1B

106080 9543260

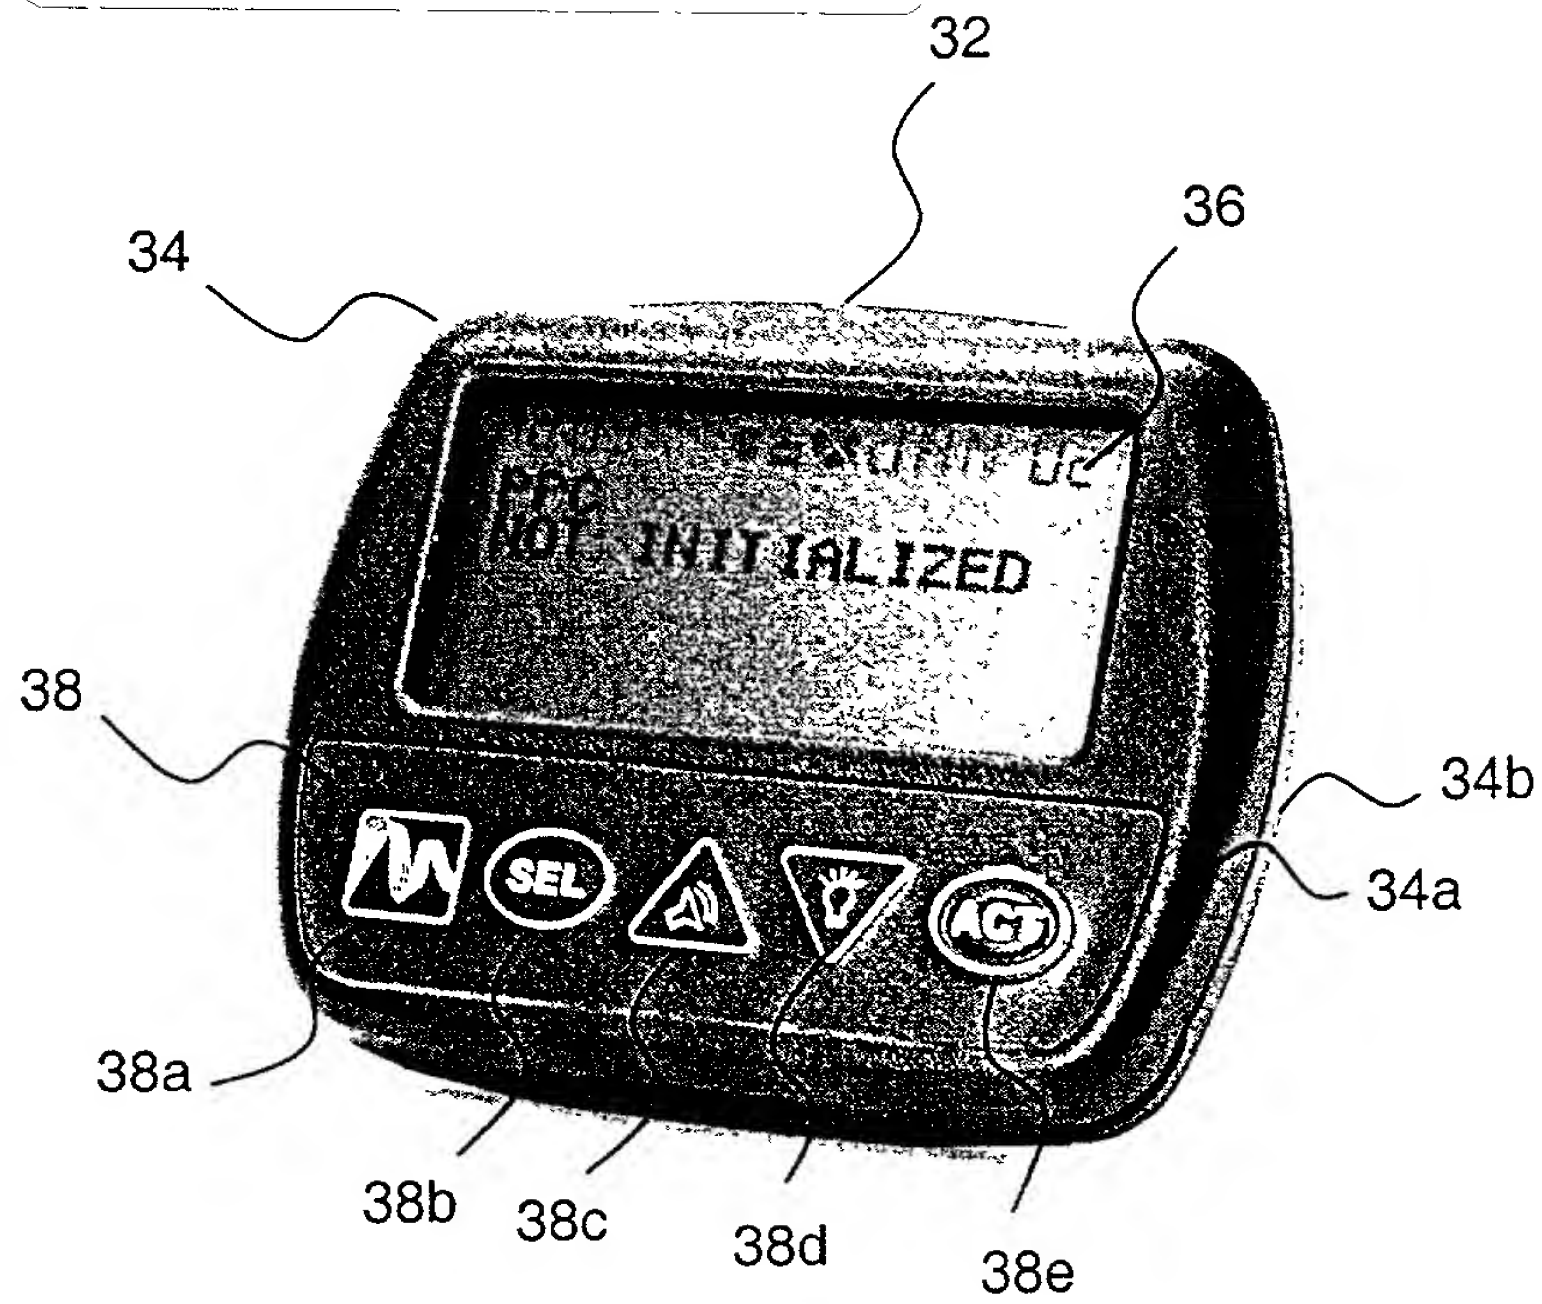


FIGURE 2

0936156-0001
T.060800 9618360

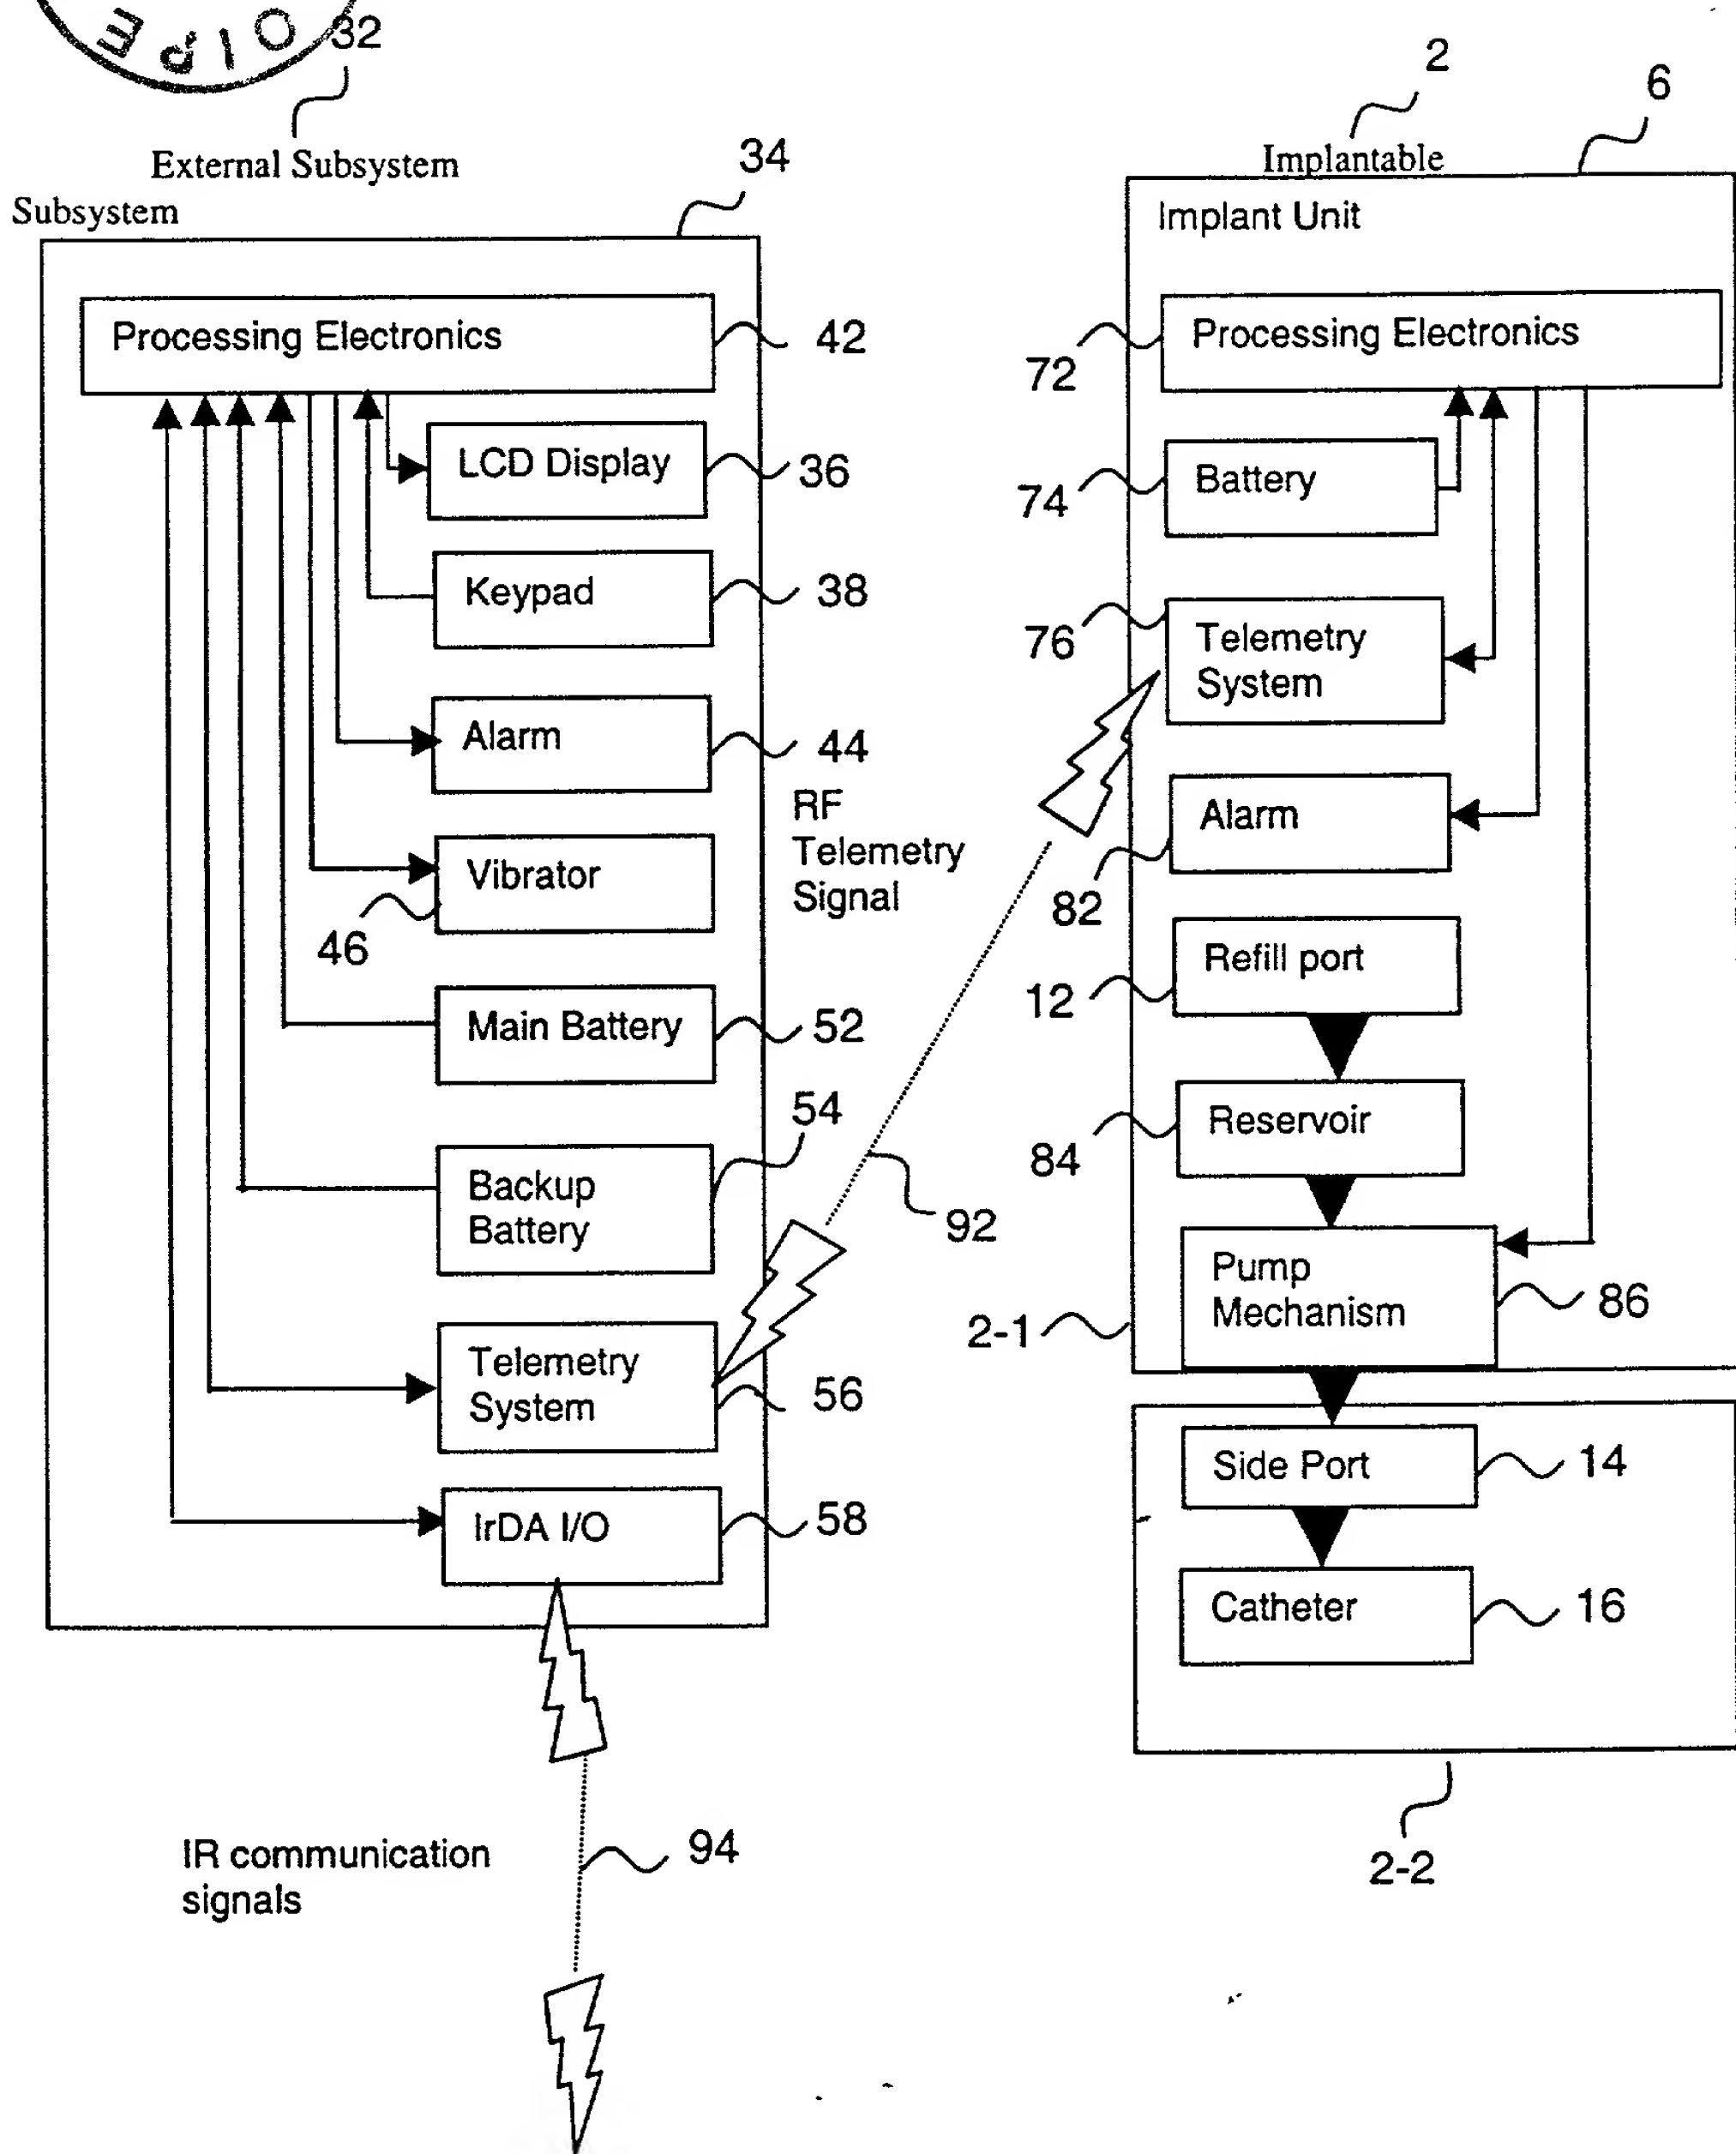


FIGURE 3

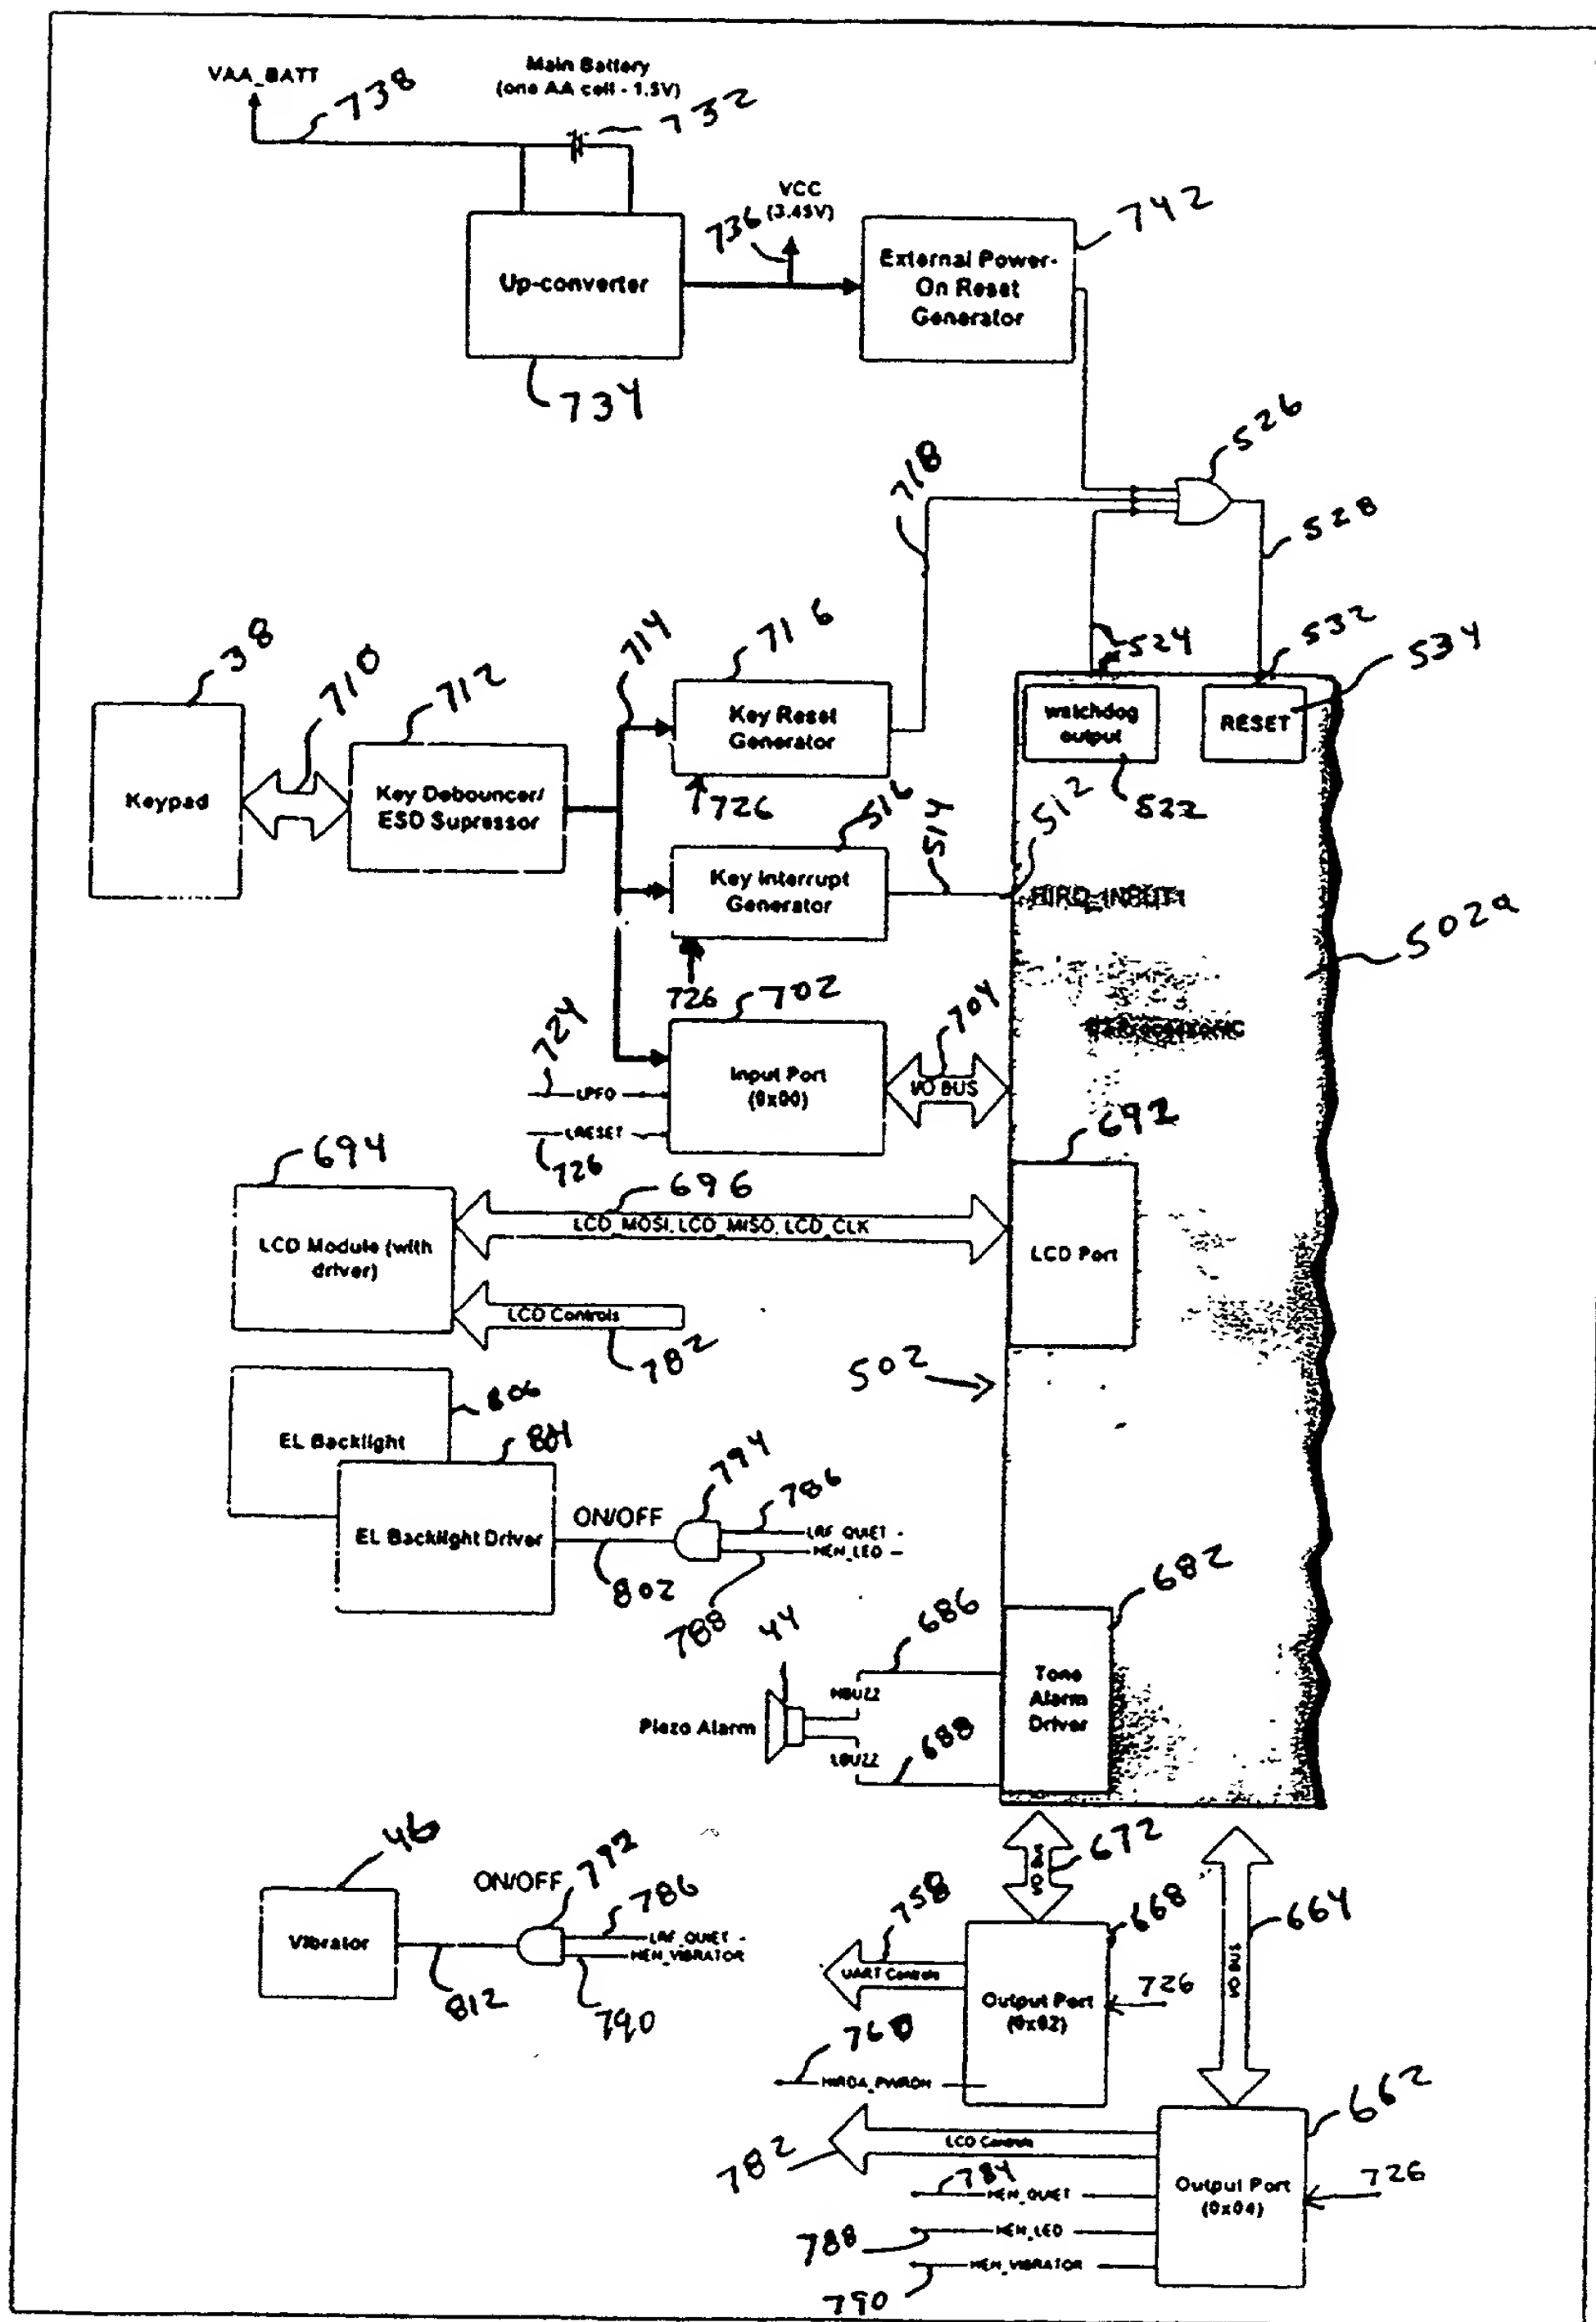


FIGURE 4a

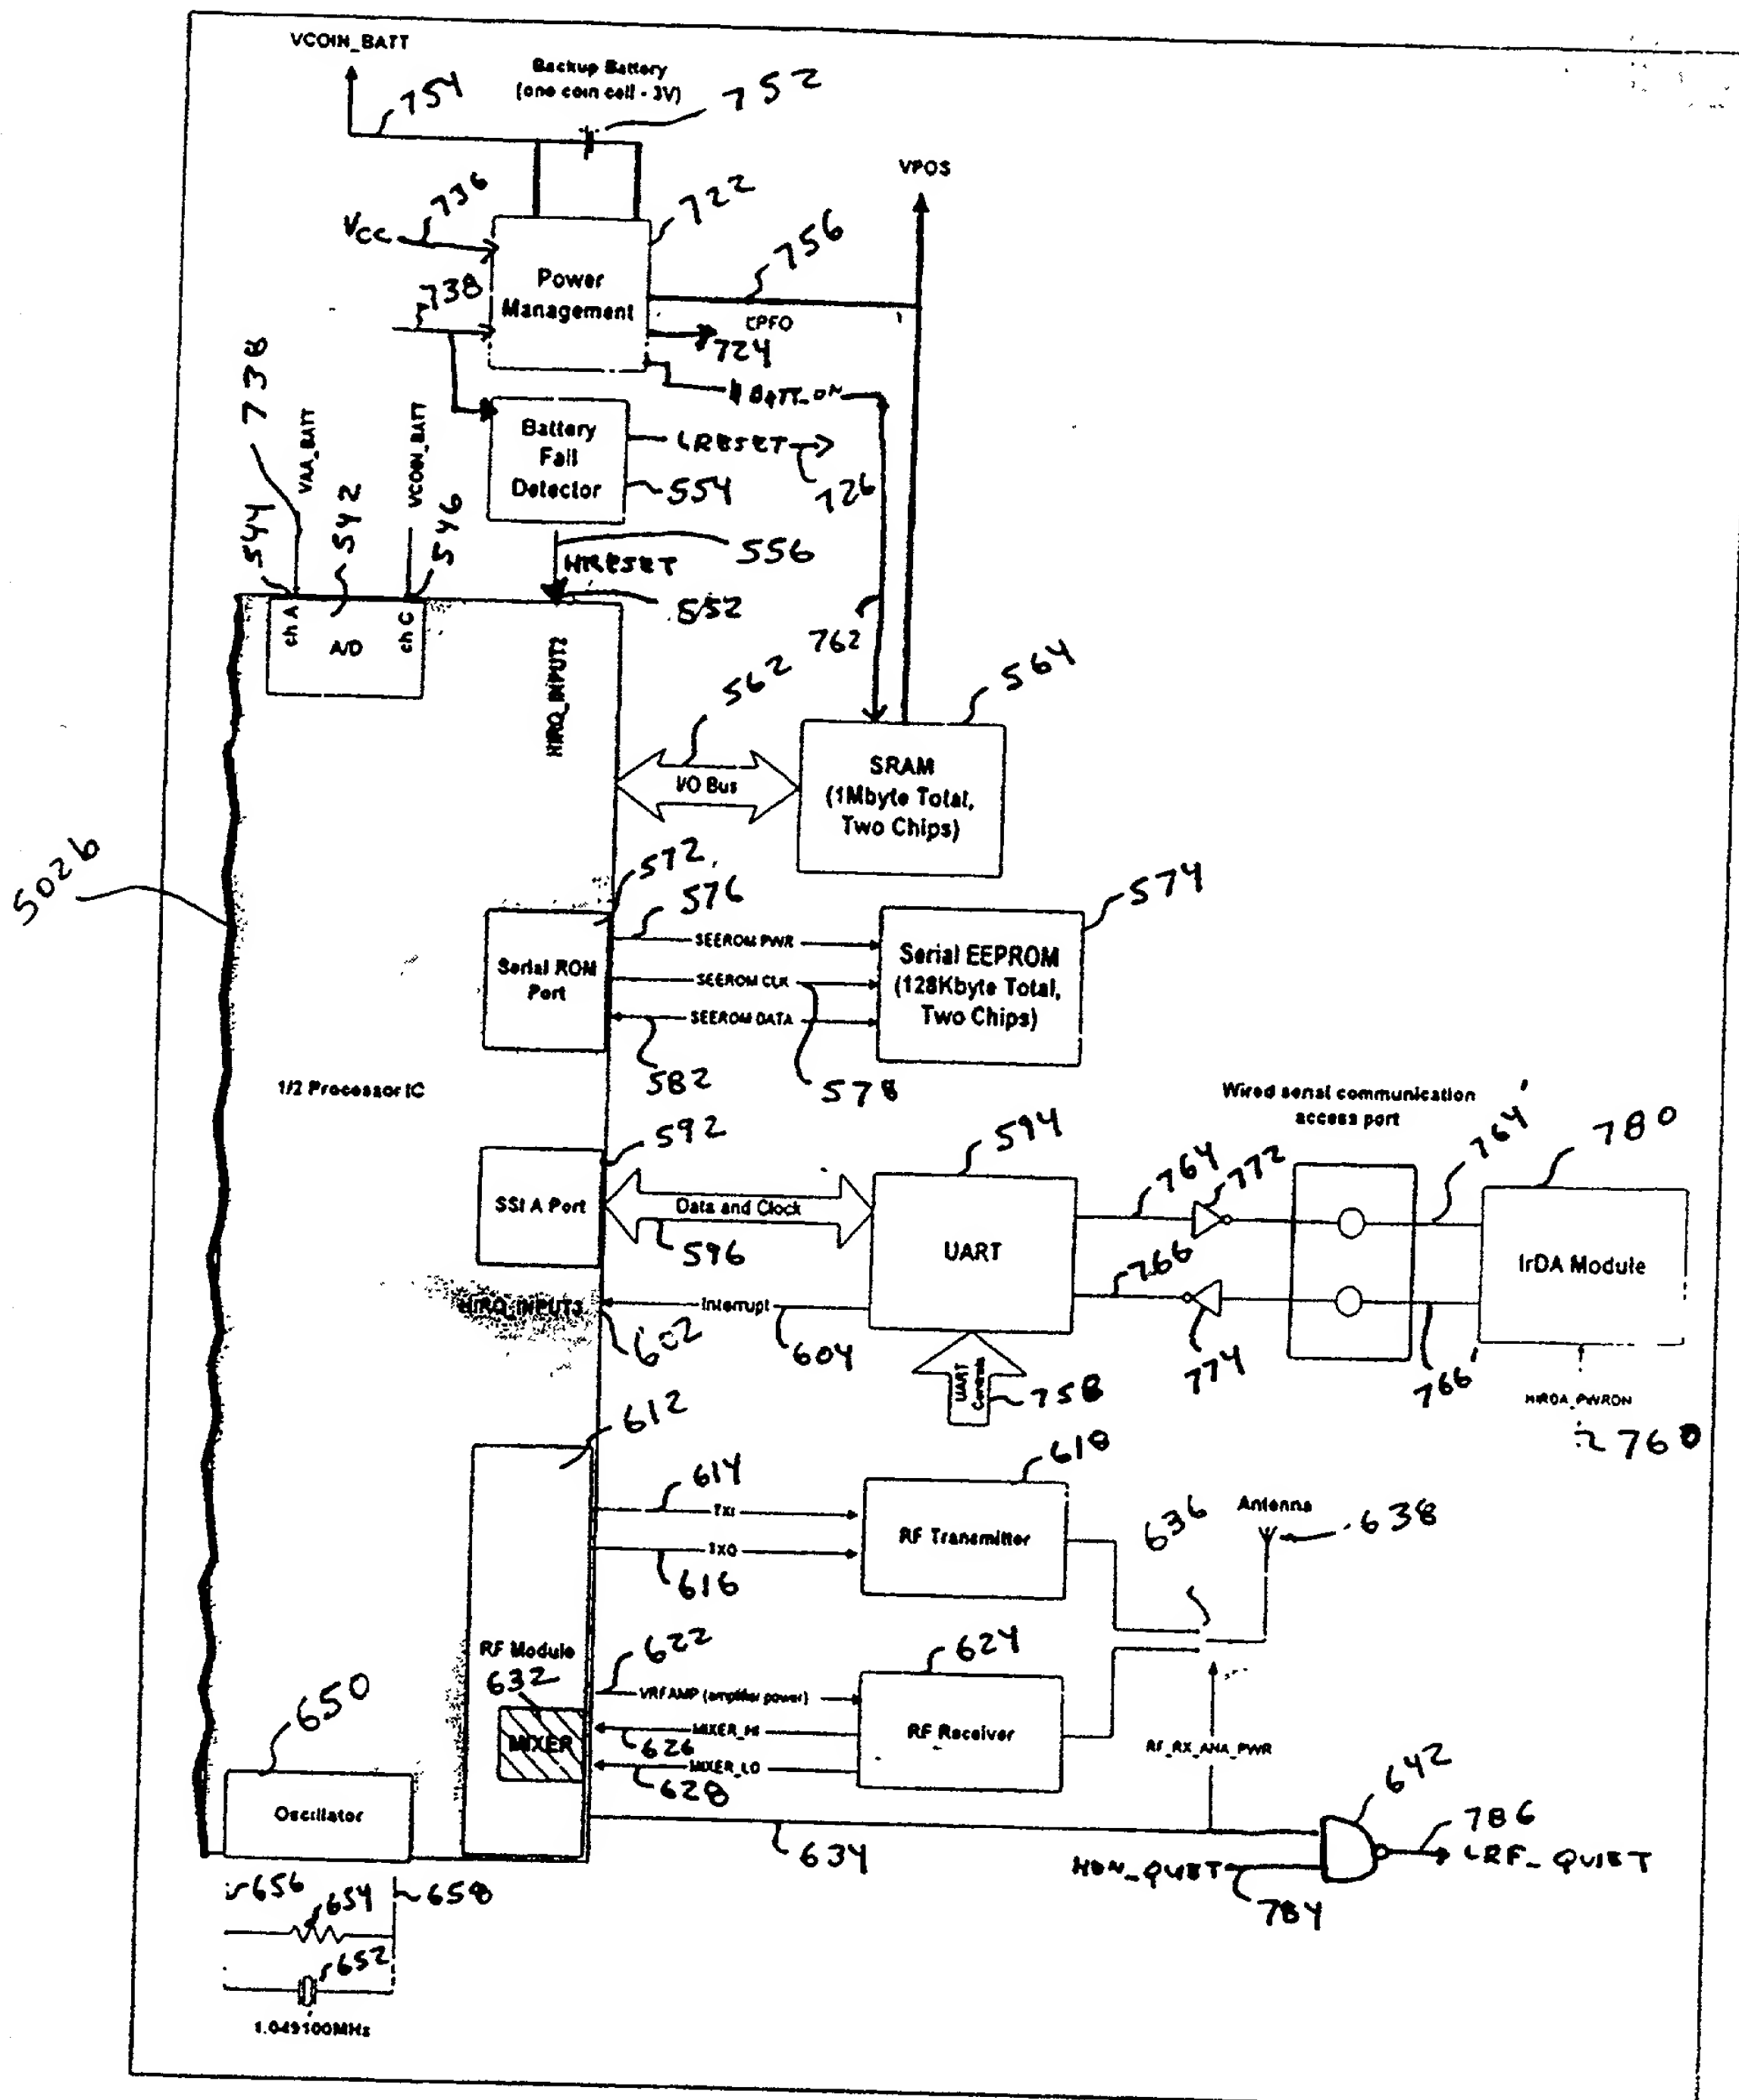


FIGURE 4b

- 88:88 ⇒ Time of Day
 8 ⇒ Battery
 8 ⇒ Alarm
 8 ⇒ Reservoir Volume Level
 8 ⇒ Delivery (Bolus/Basal)
 888 ⇒ Month
 88 ⇒ Date of Month

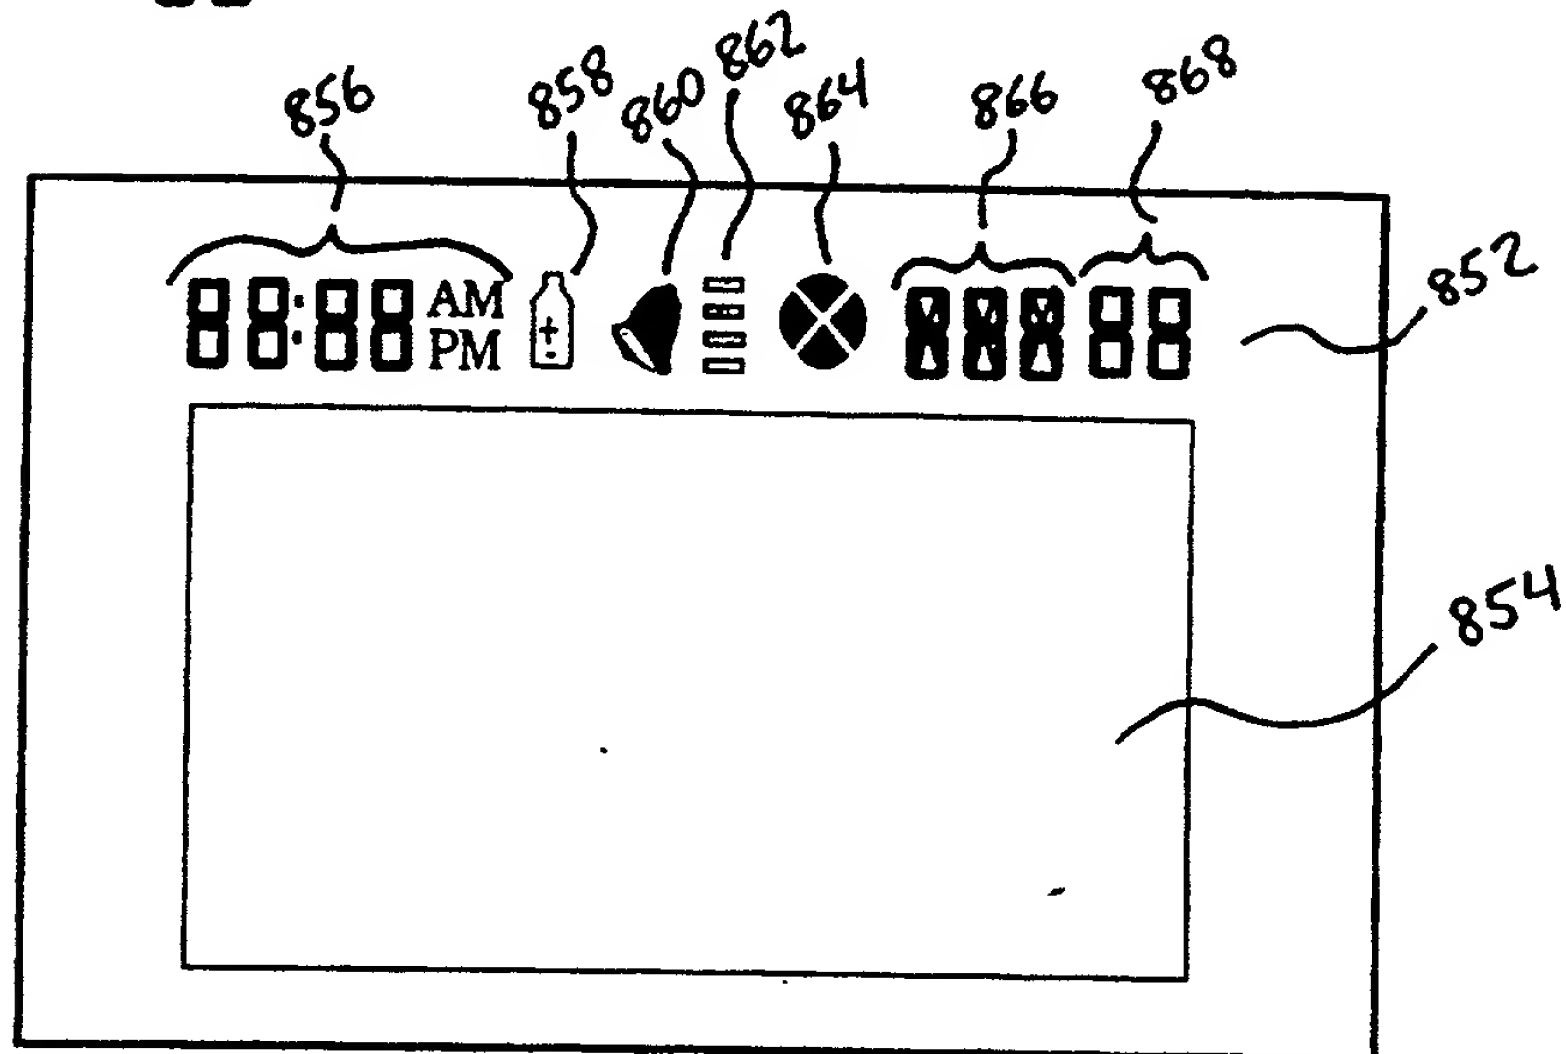


FIGURE 5

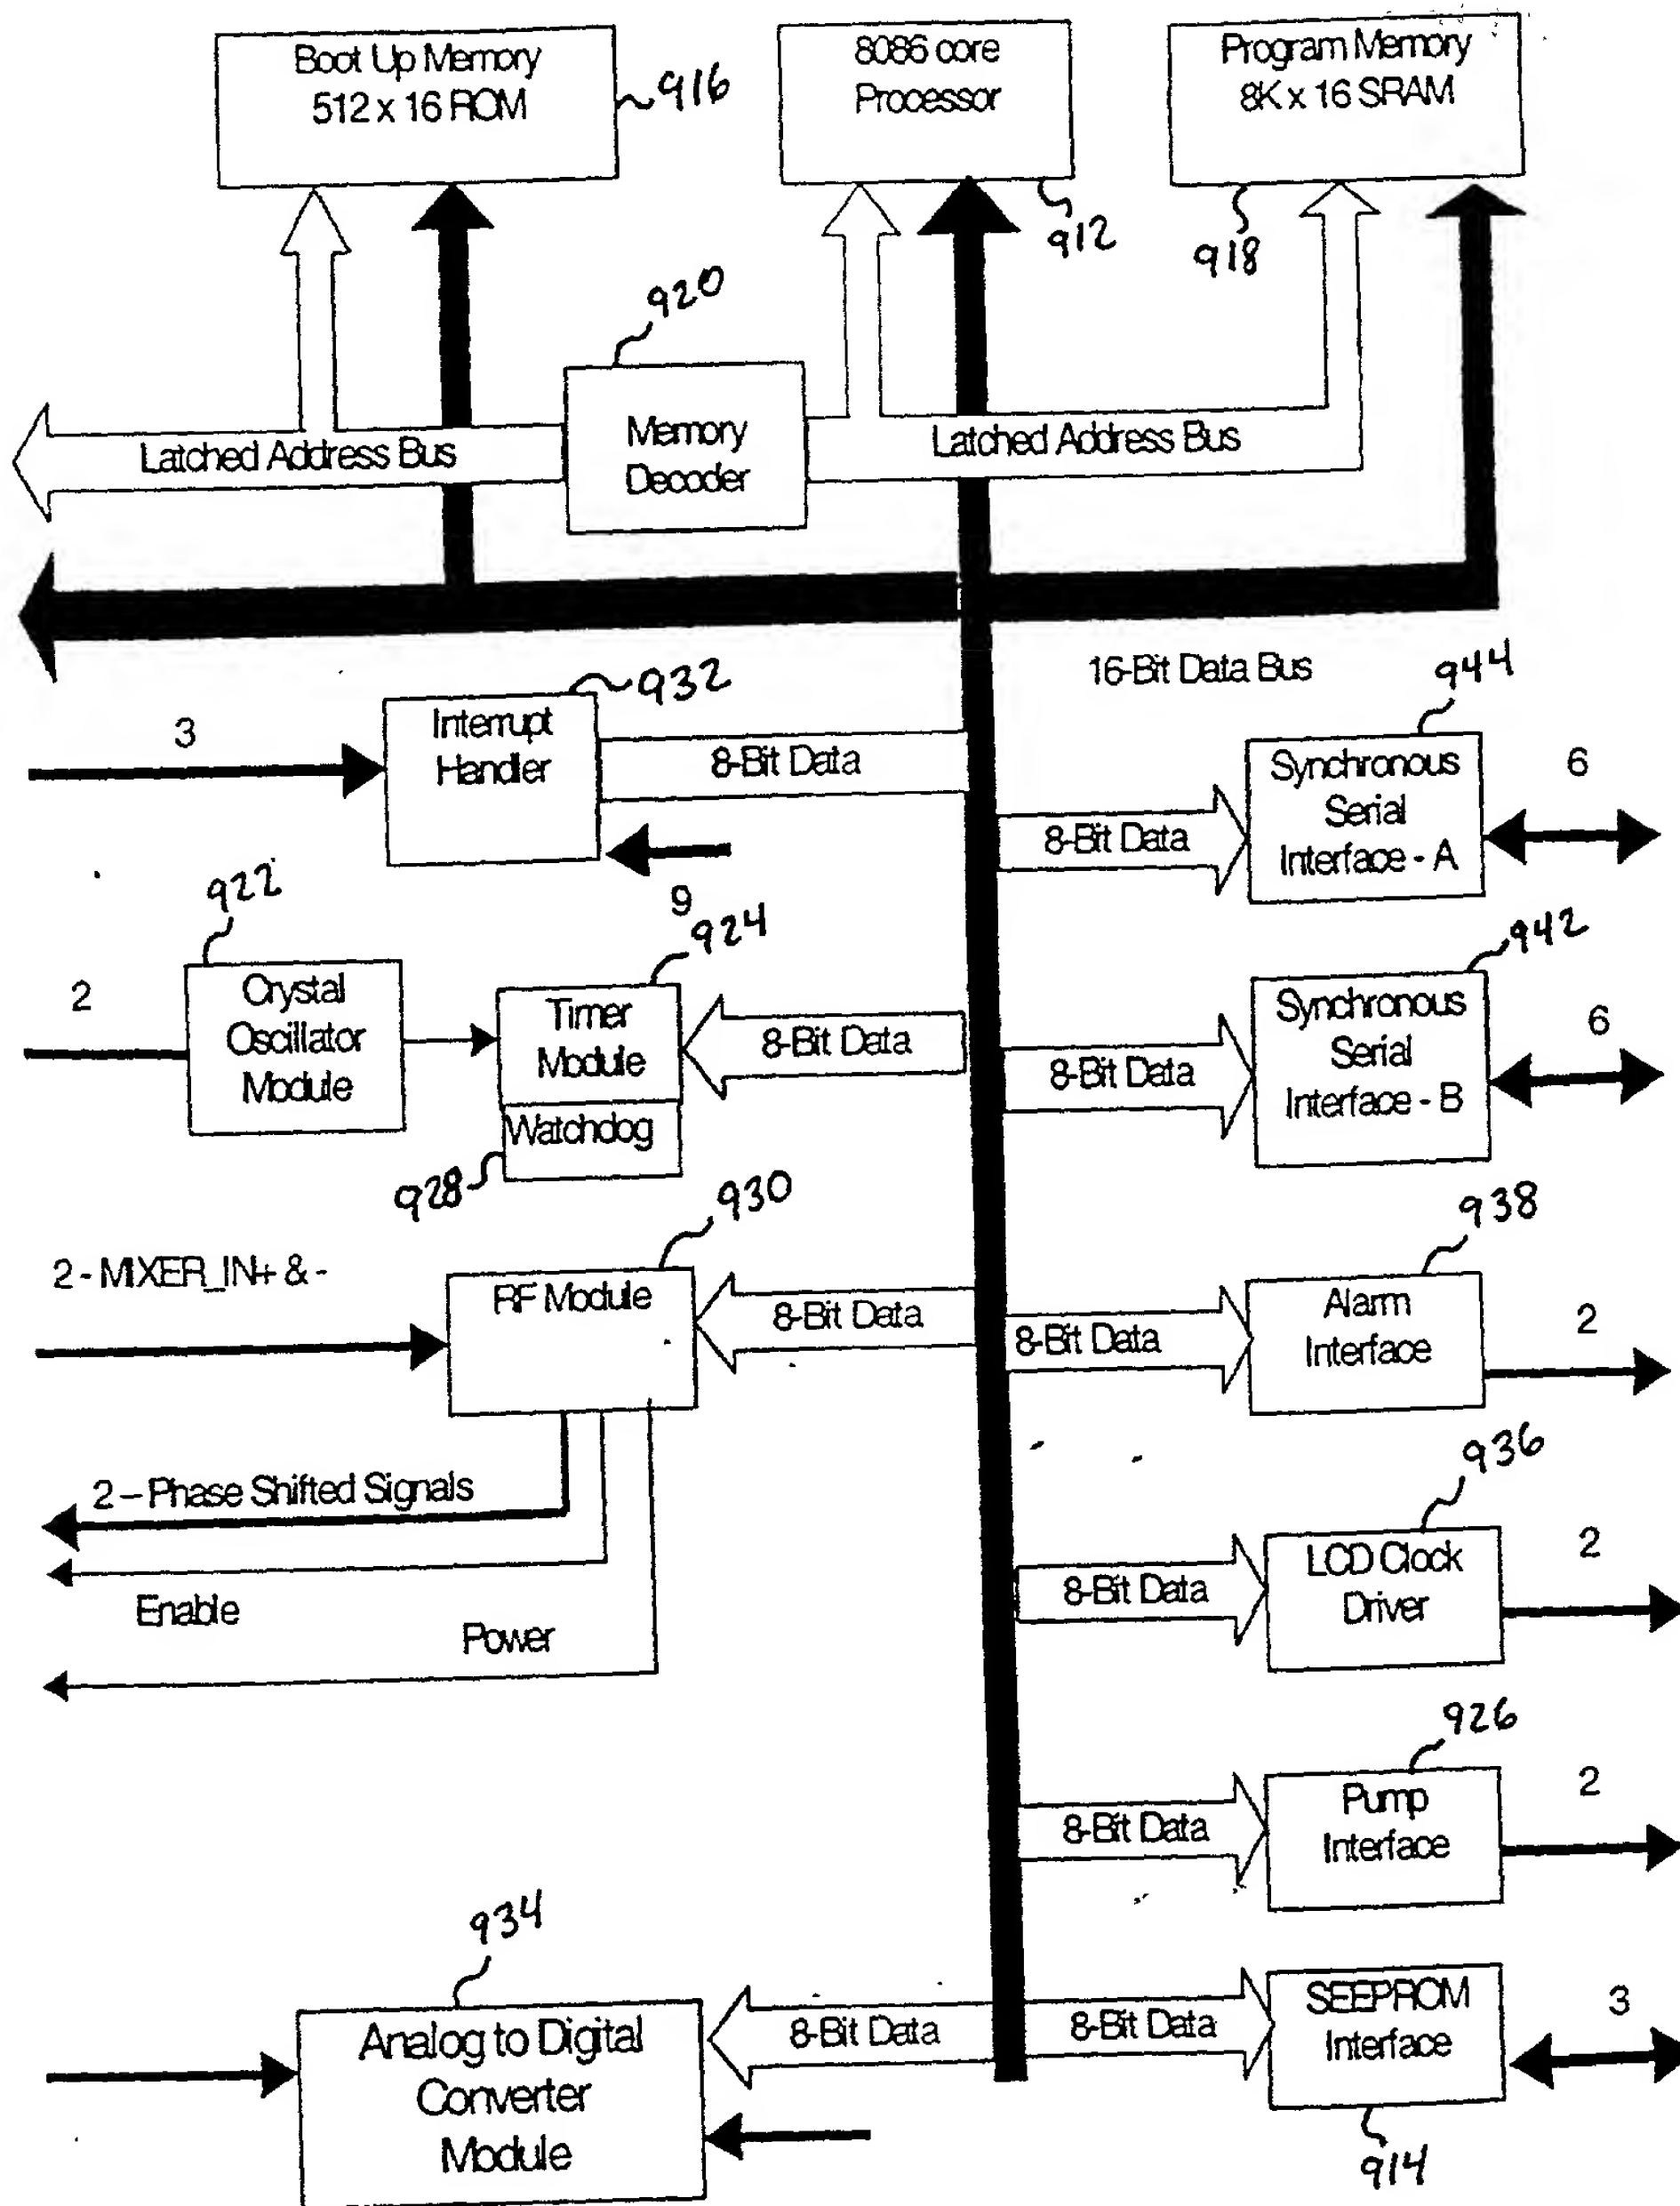


Figure 6

902

105080-05 FEB 95

Main Menu


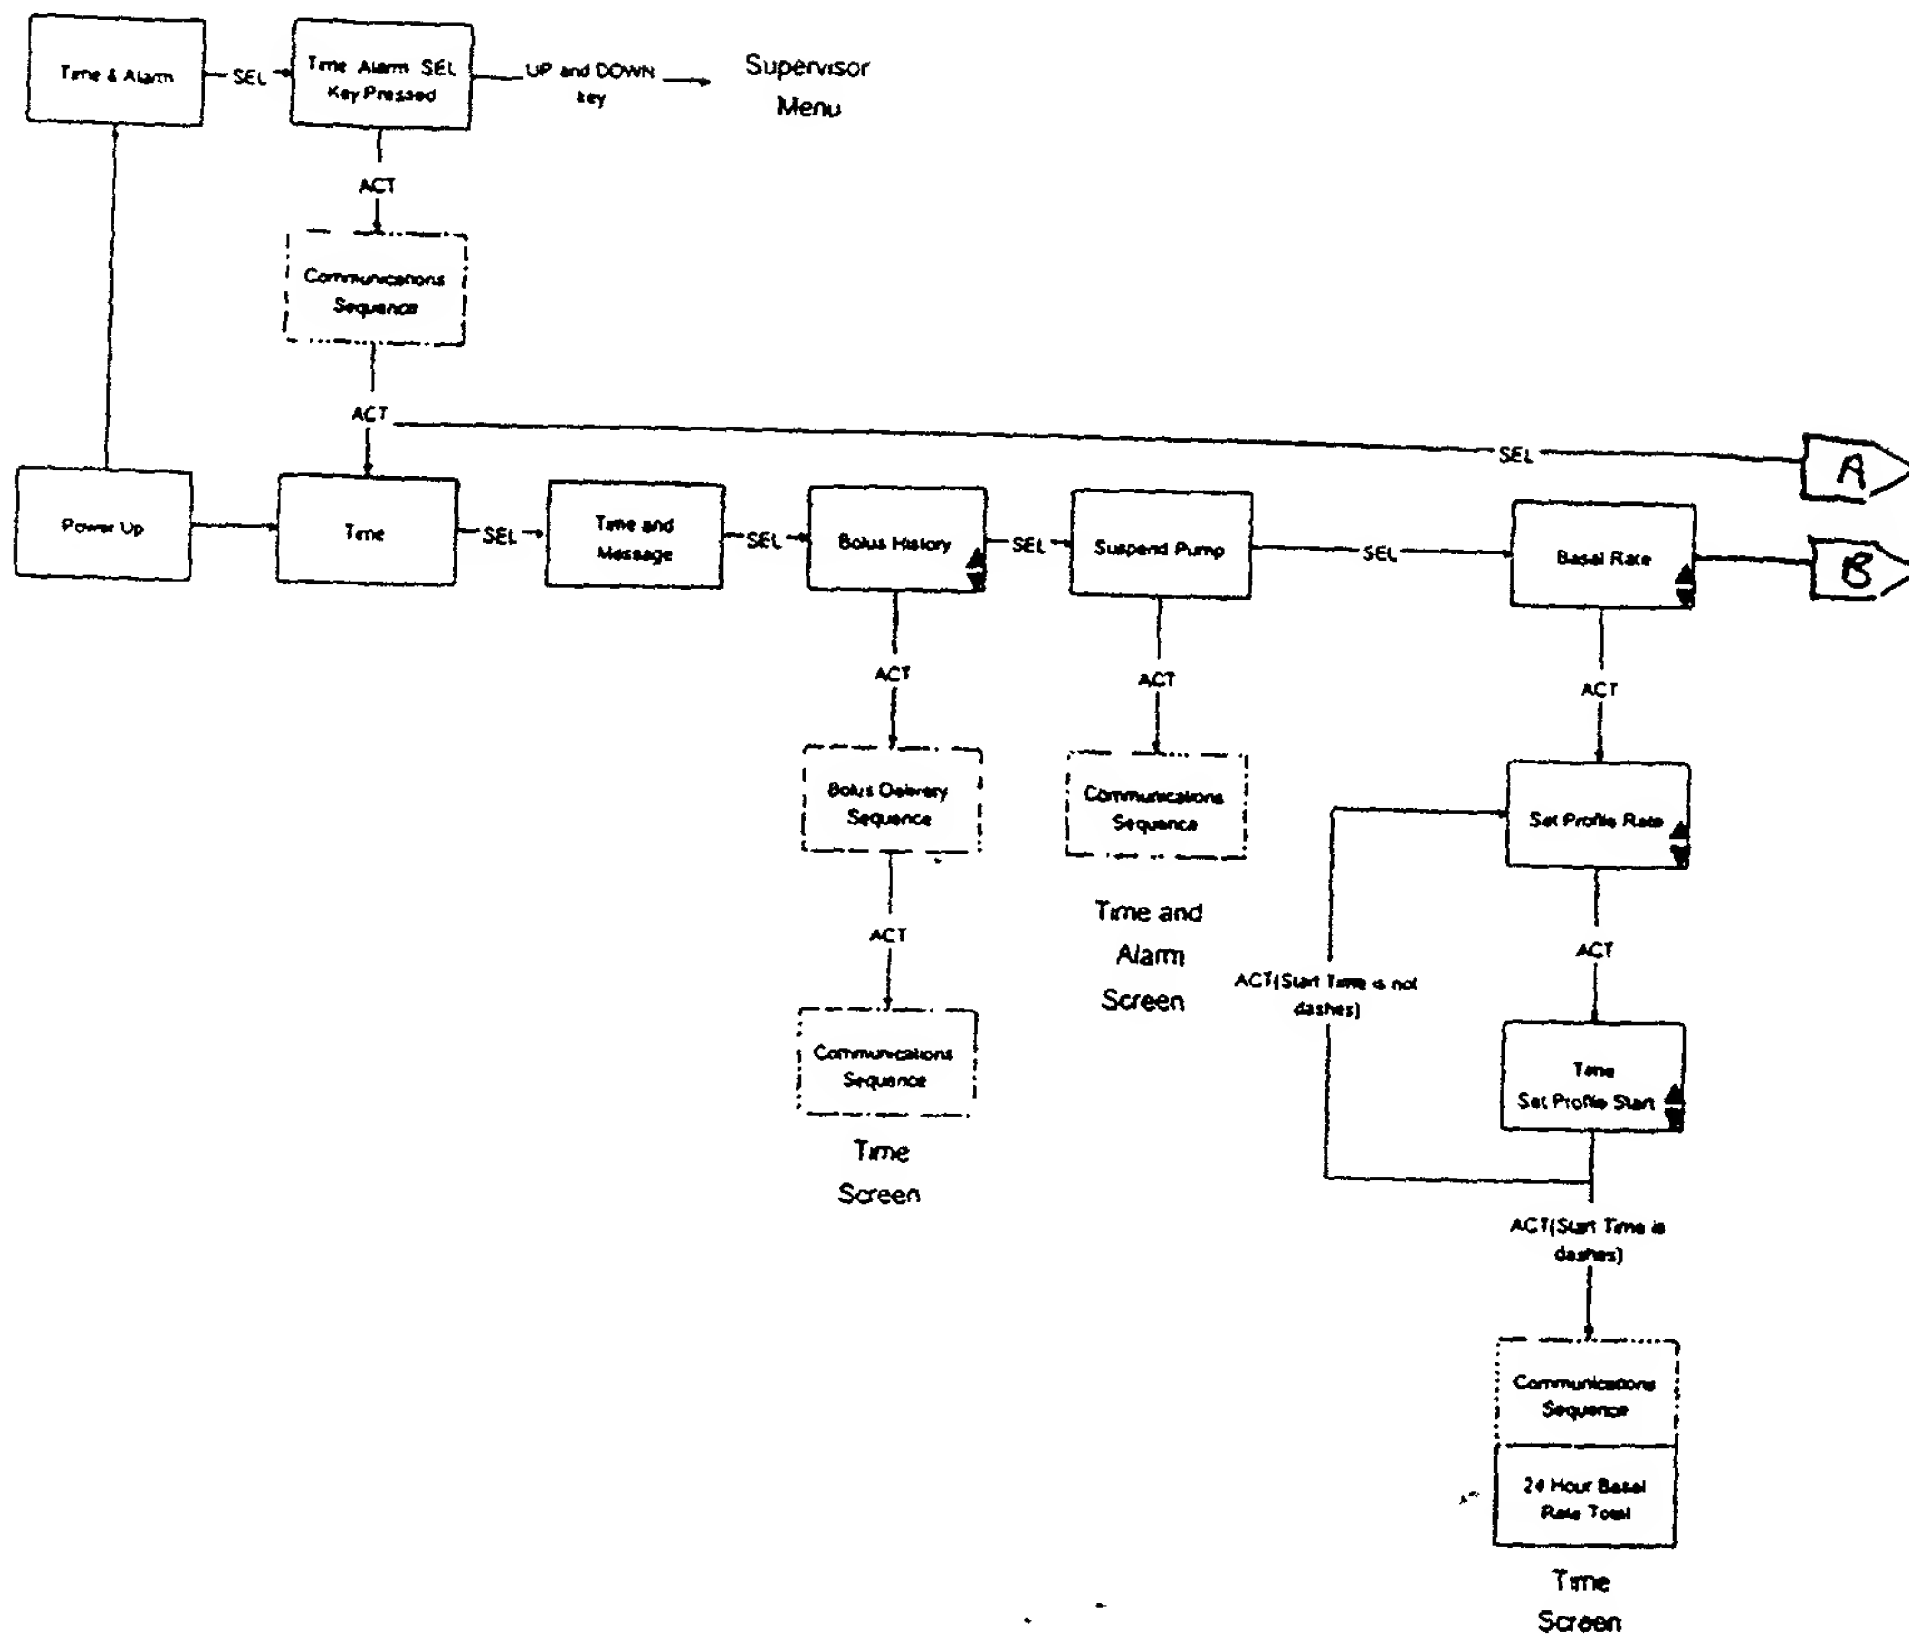


FIGURE 7a

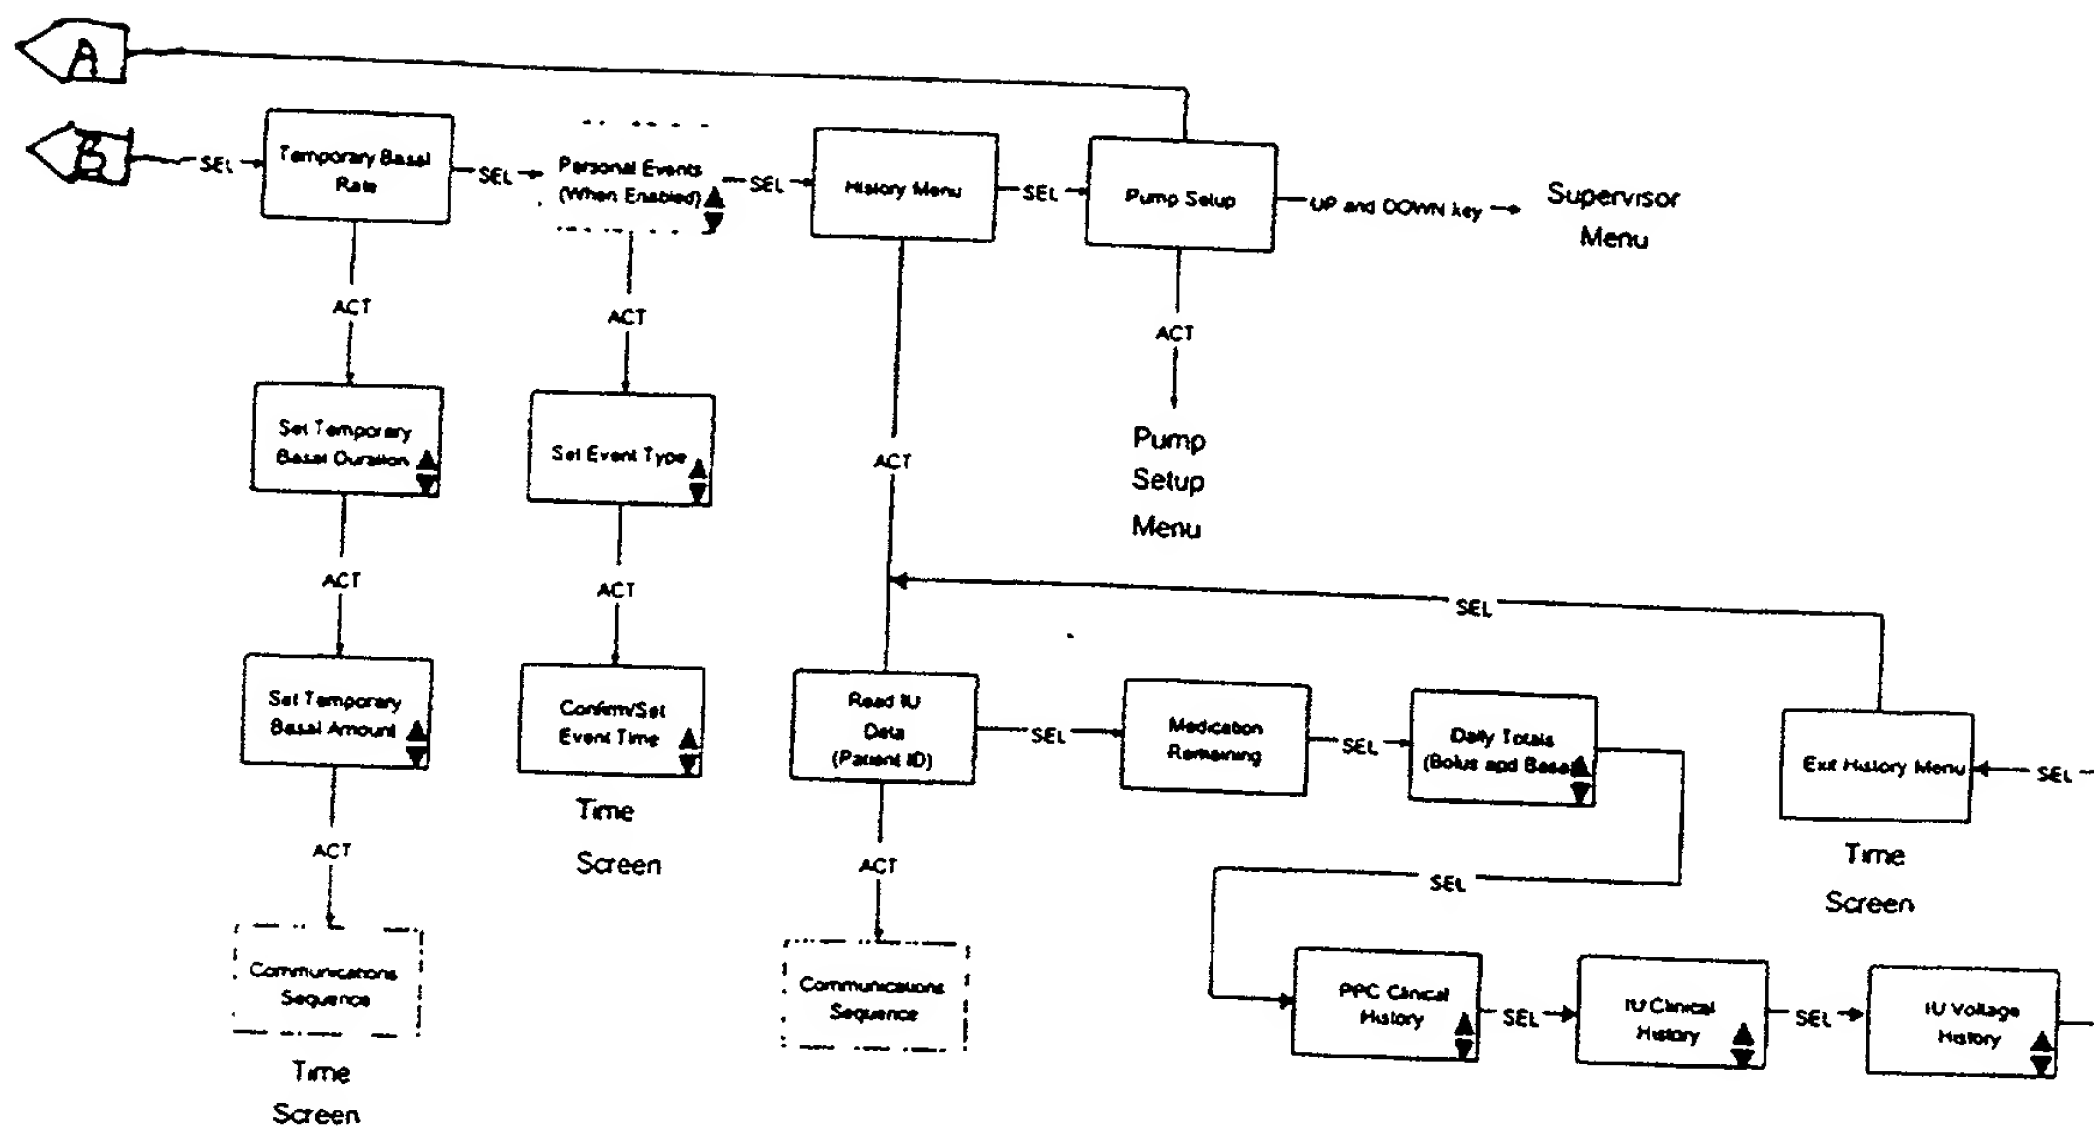

If the Communications Sequence on the History Menu is successful, the next screen in the menu shall be displayed

FIGURE 7b

Setup Menus

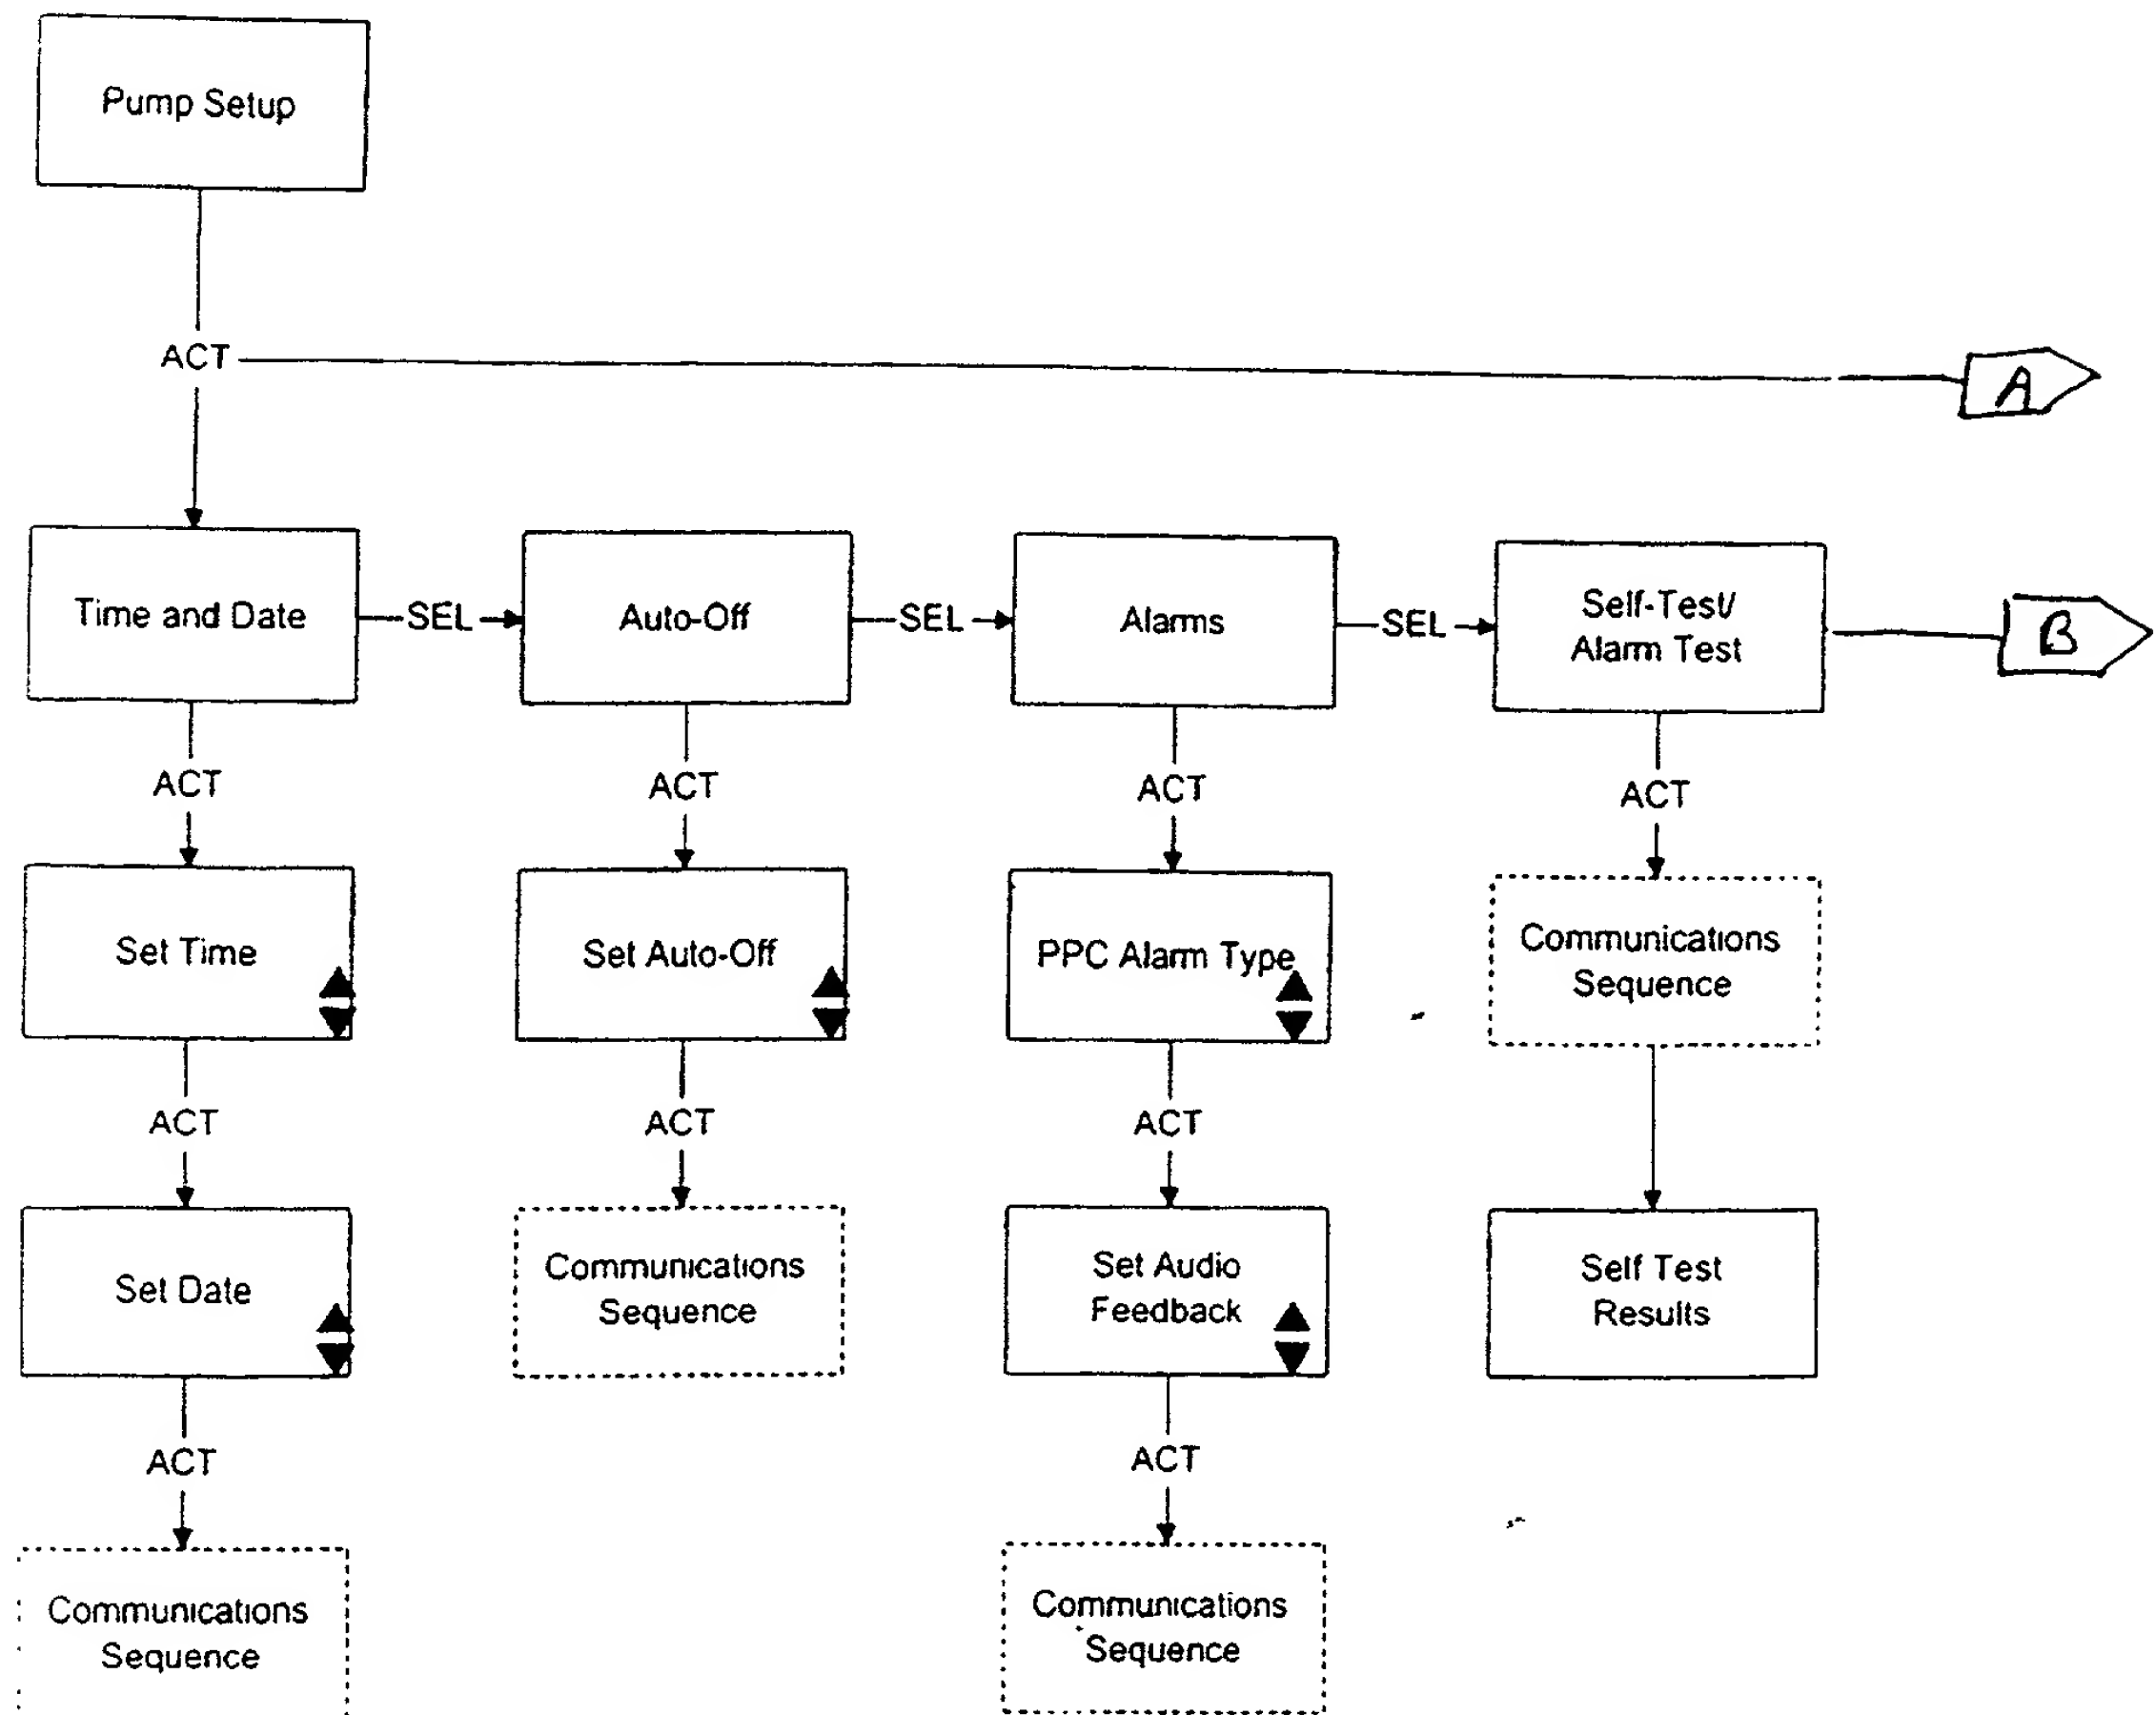


FIGURE 8a


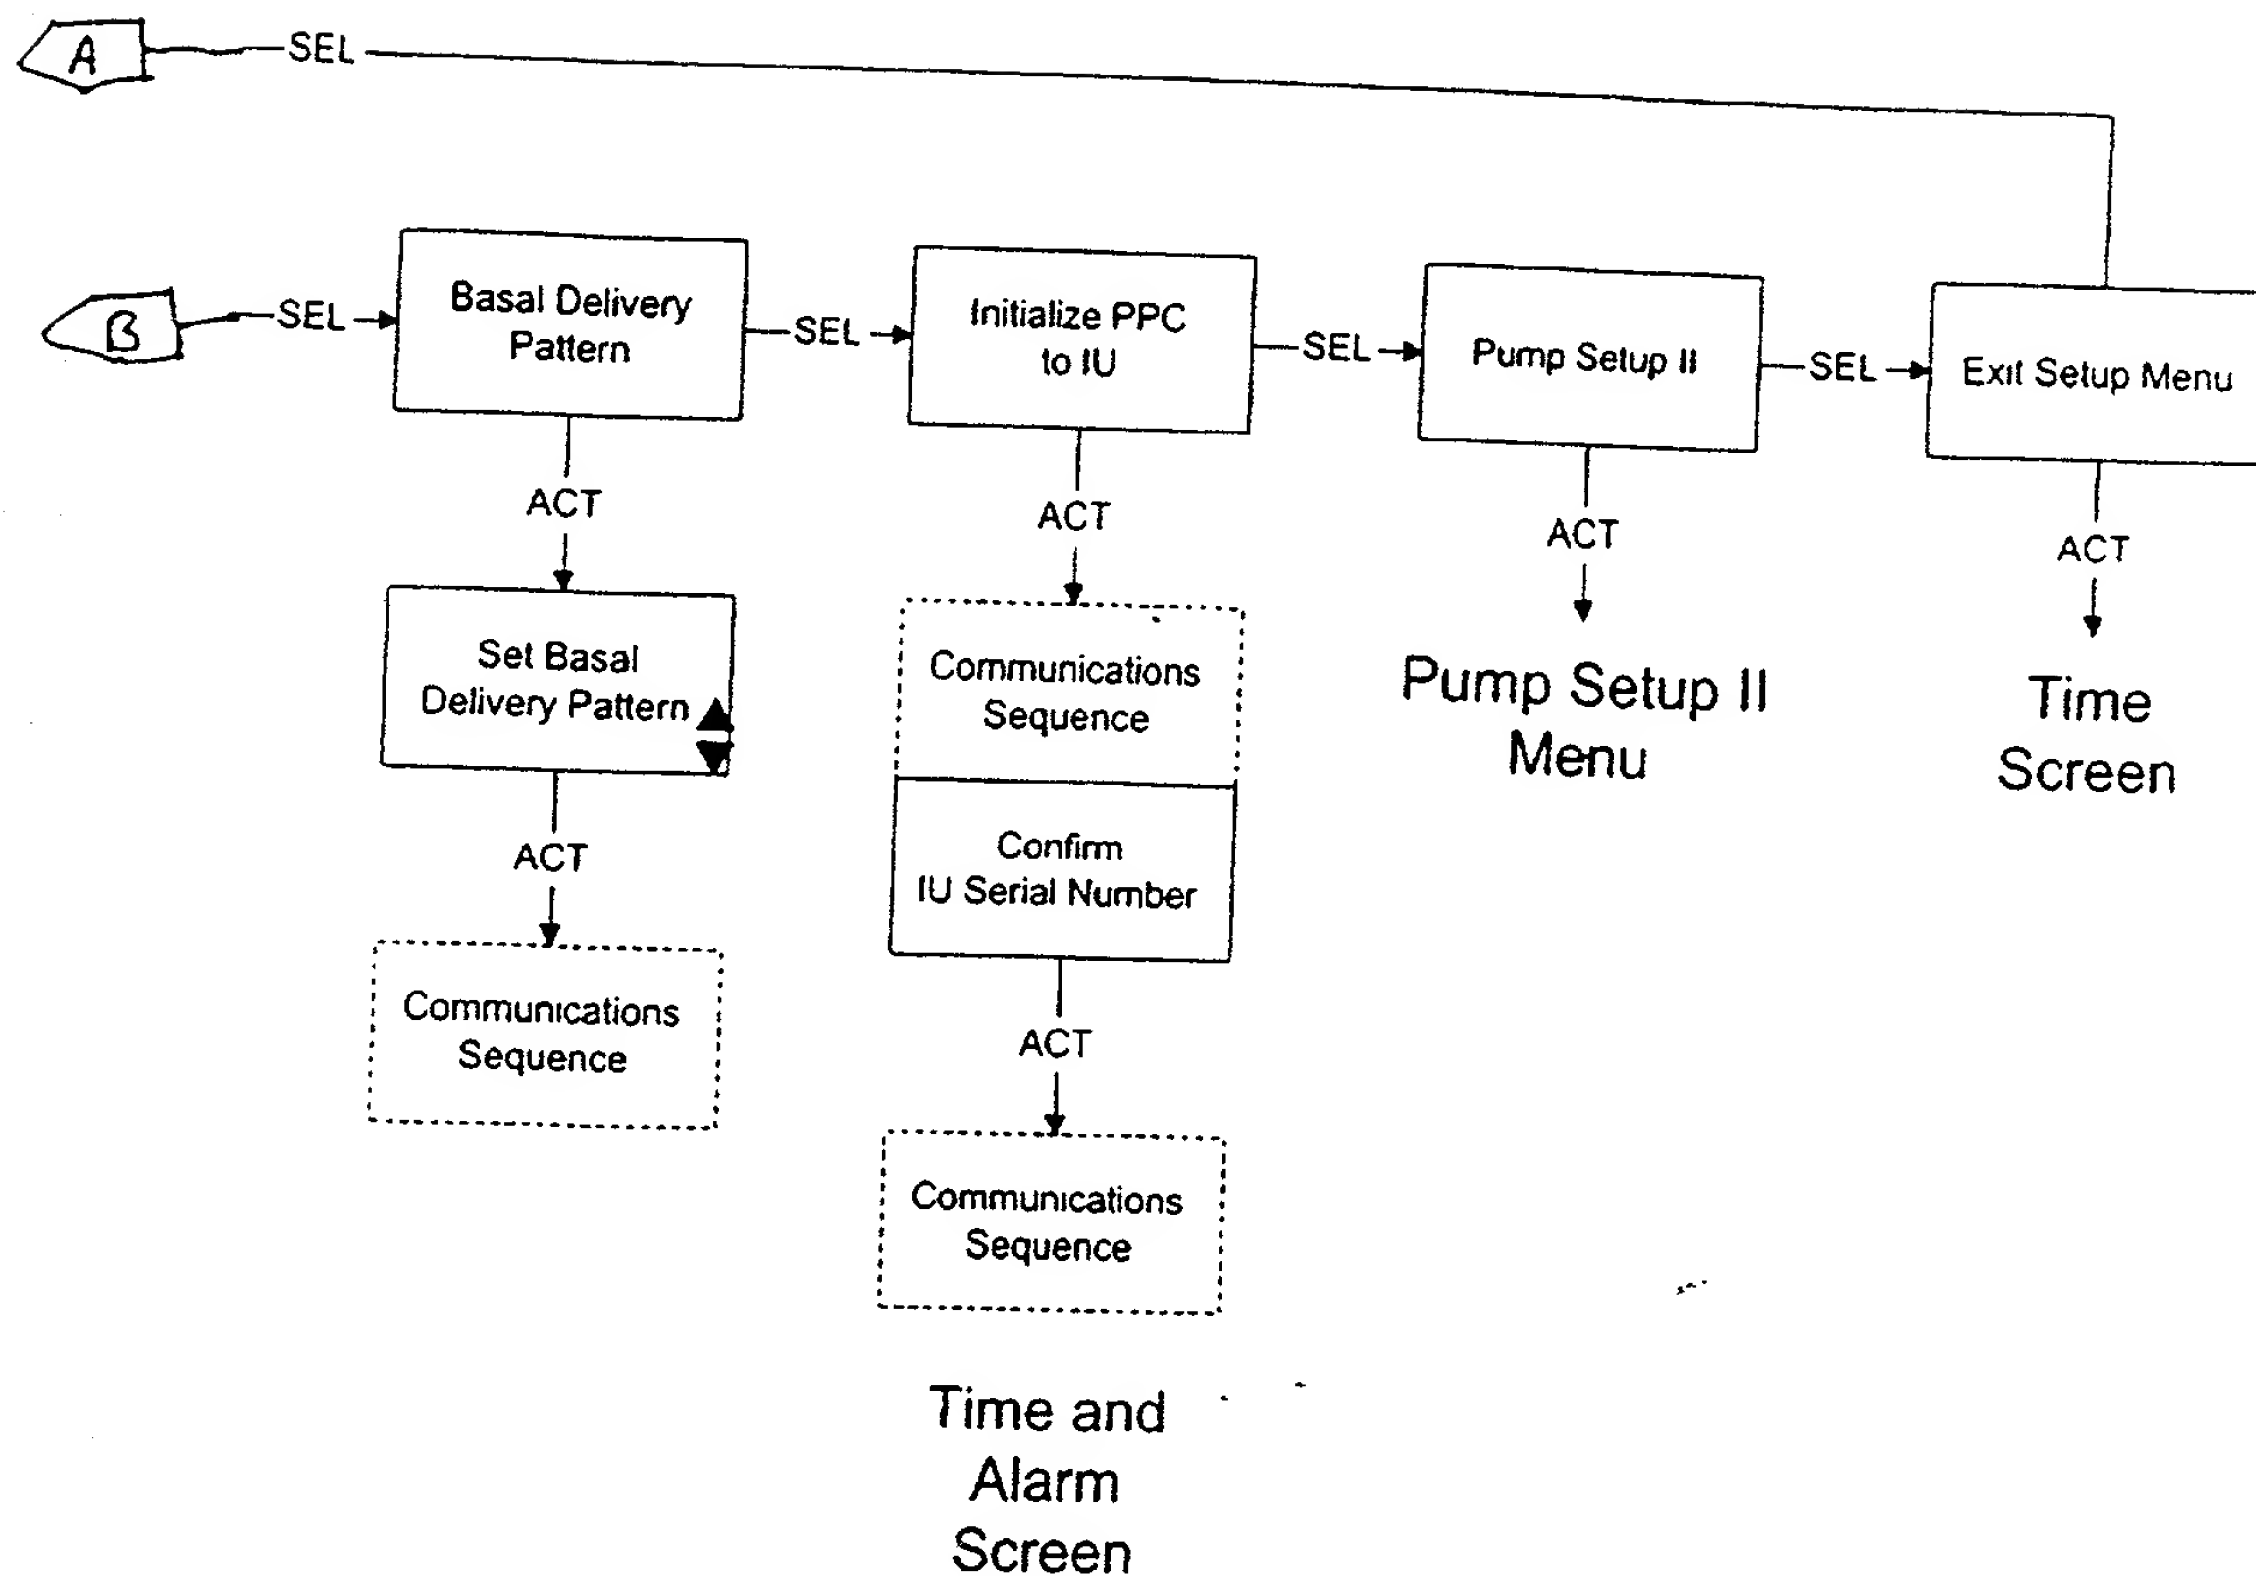


FIGURE 8b

Pump Setup II Menu

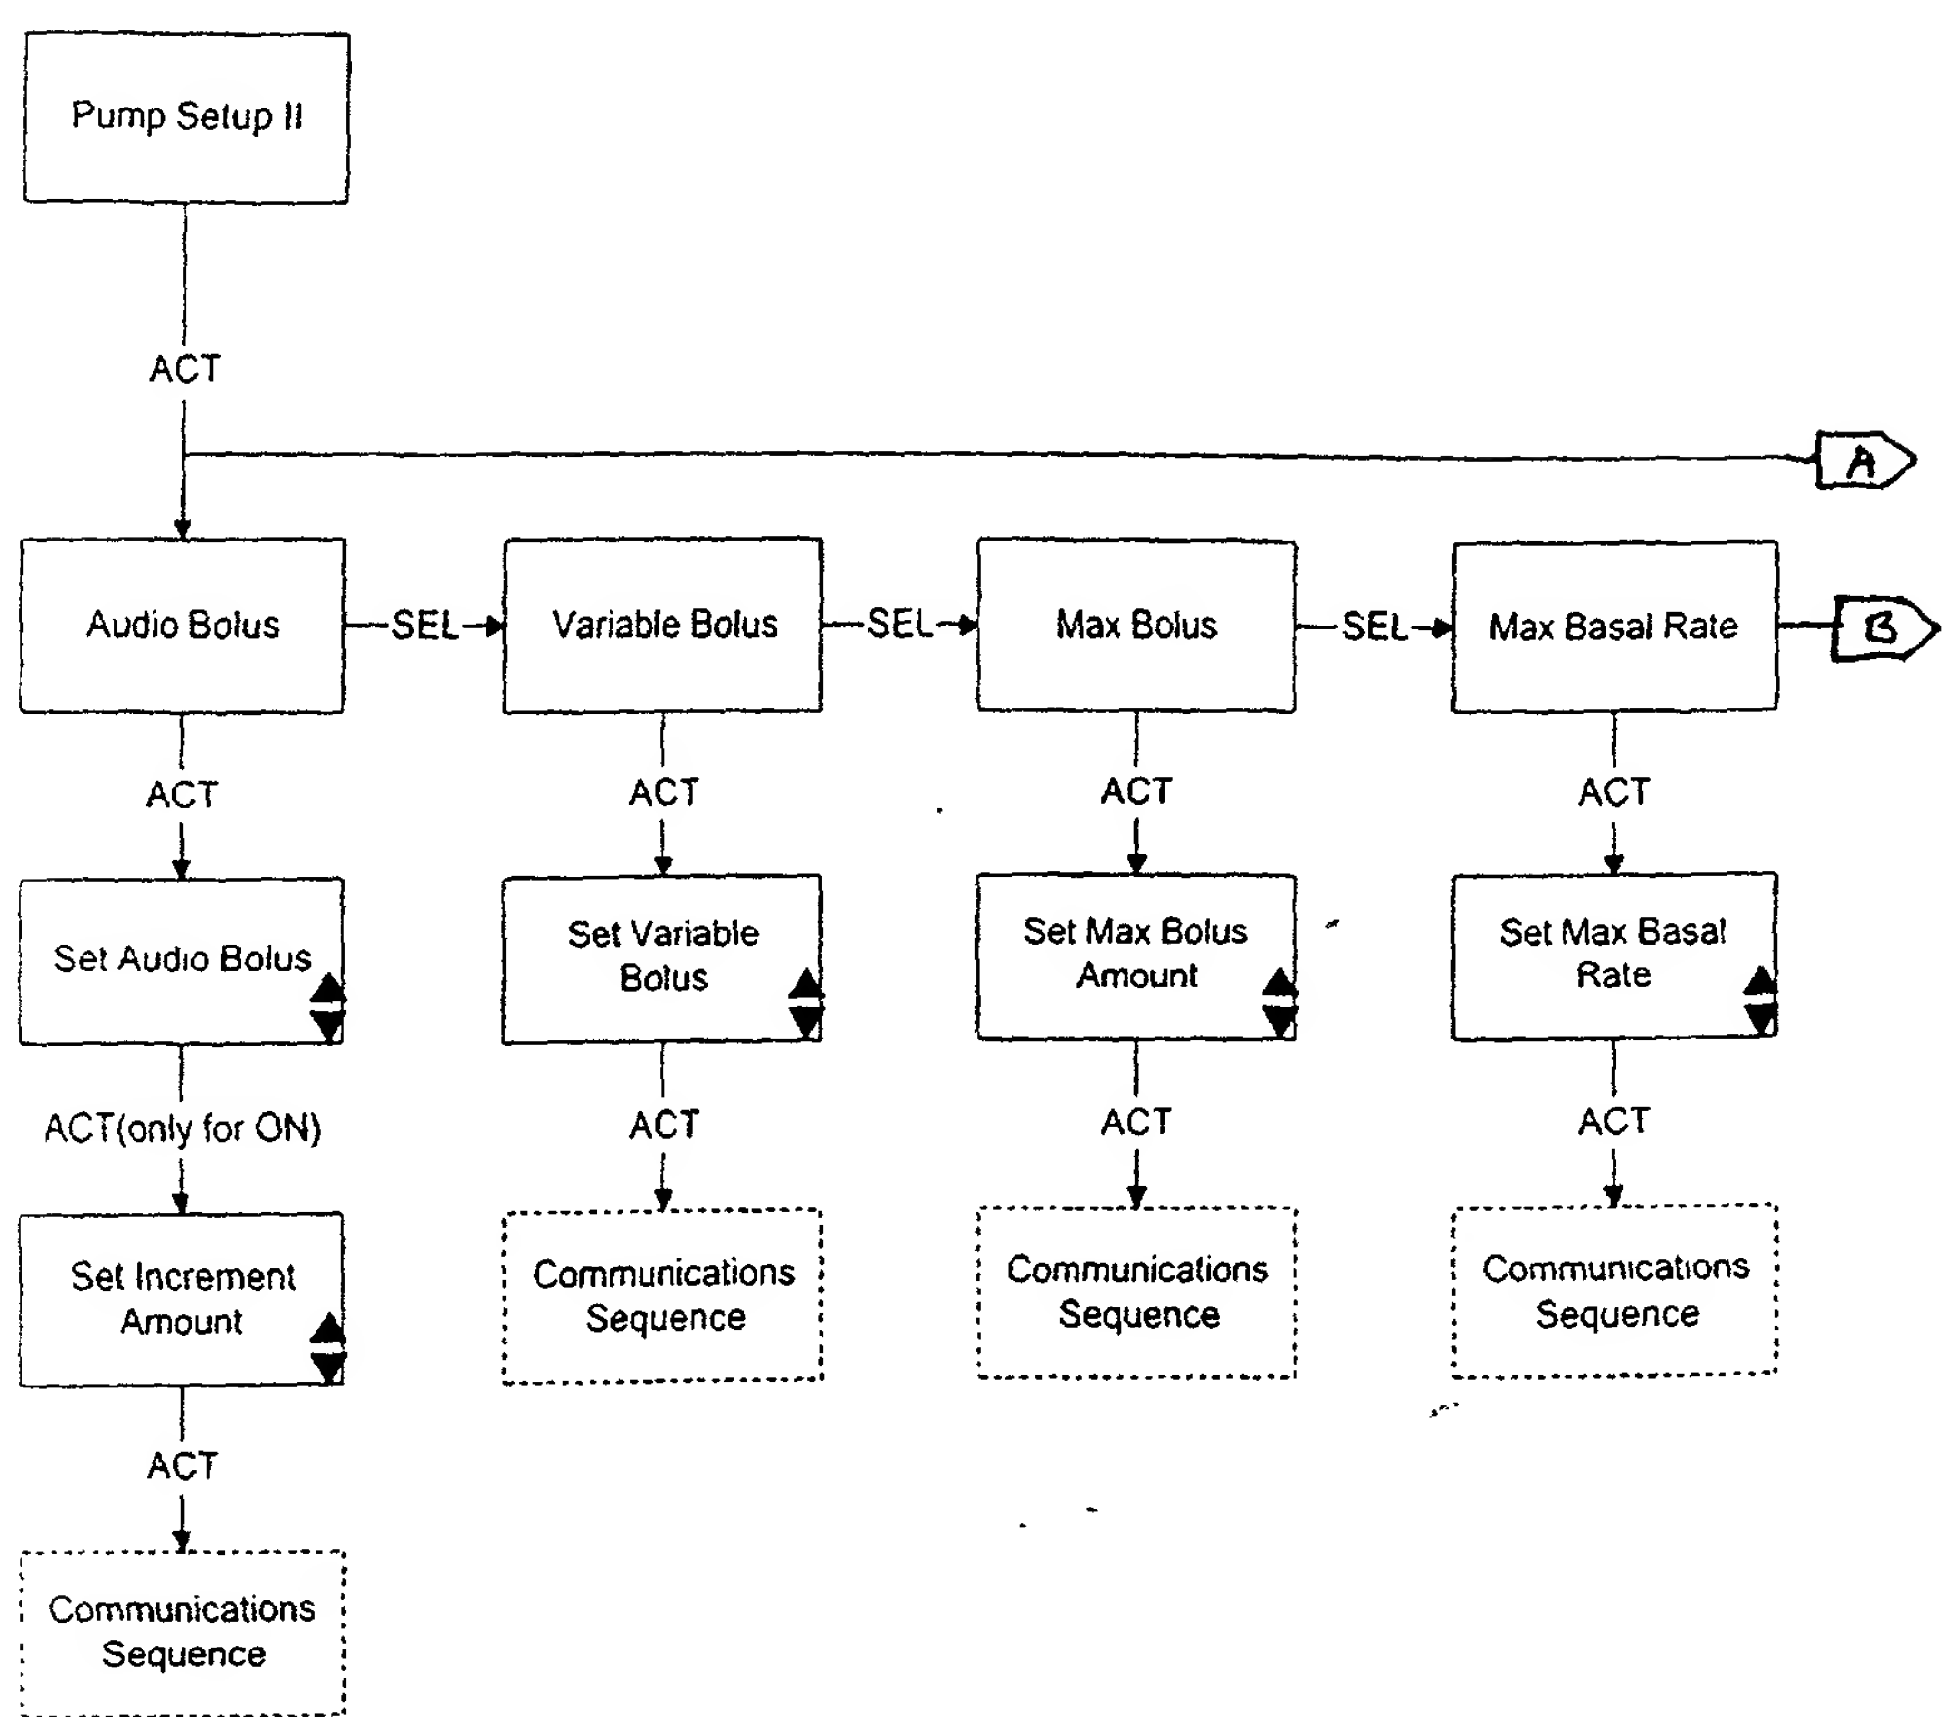

If the Communication Sequence is successful, the next screen in the menu shall be displayed.

FIGURE 9a


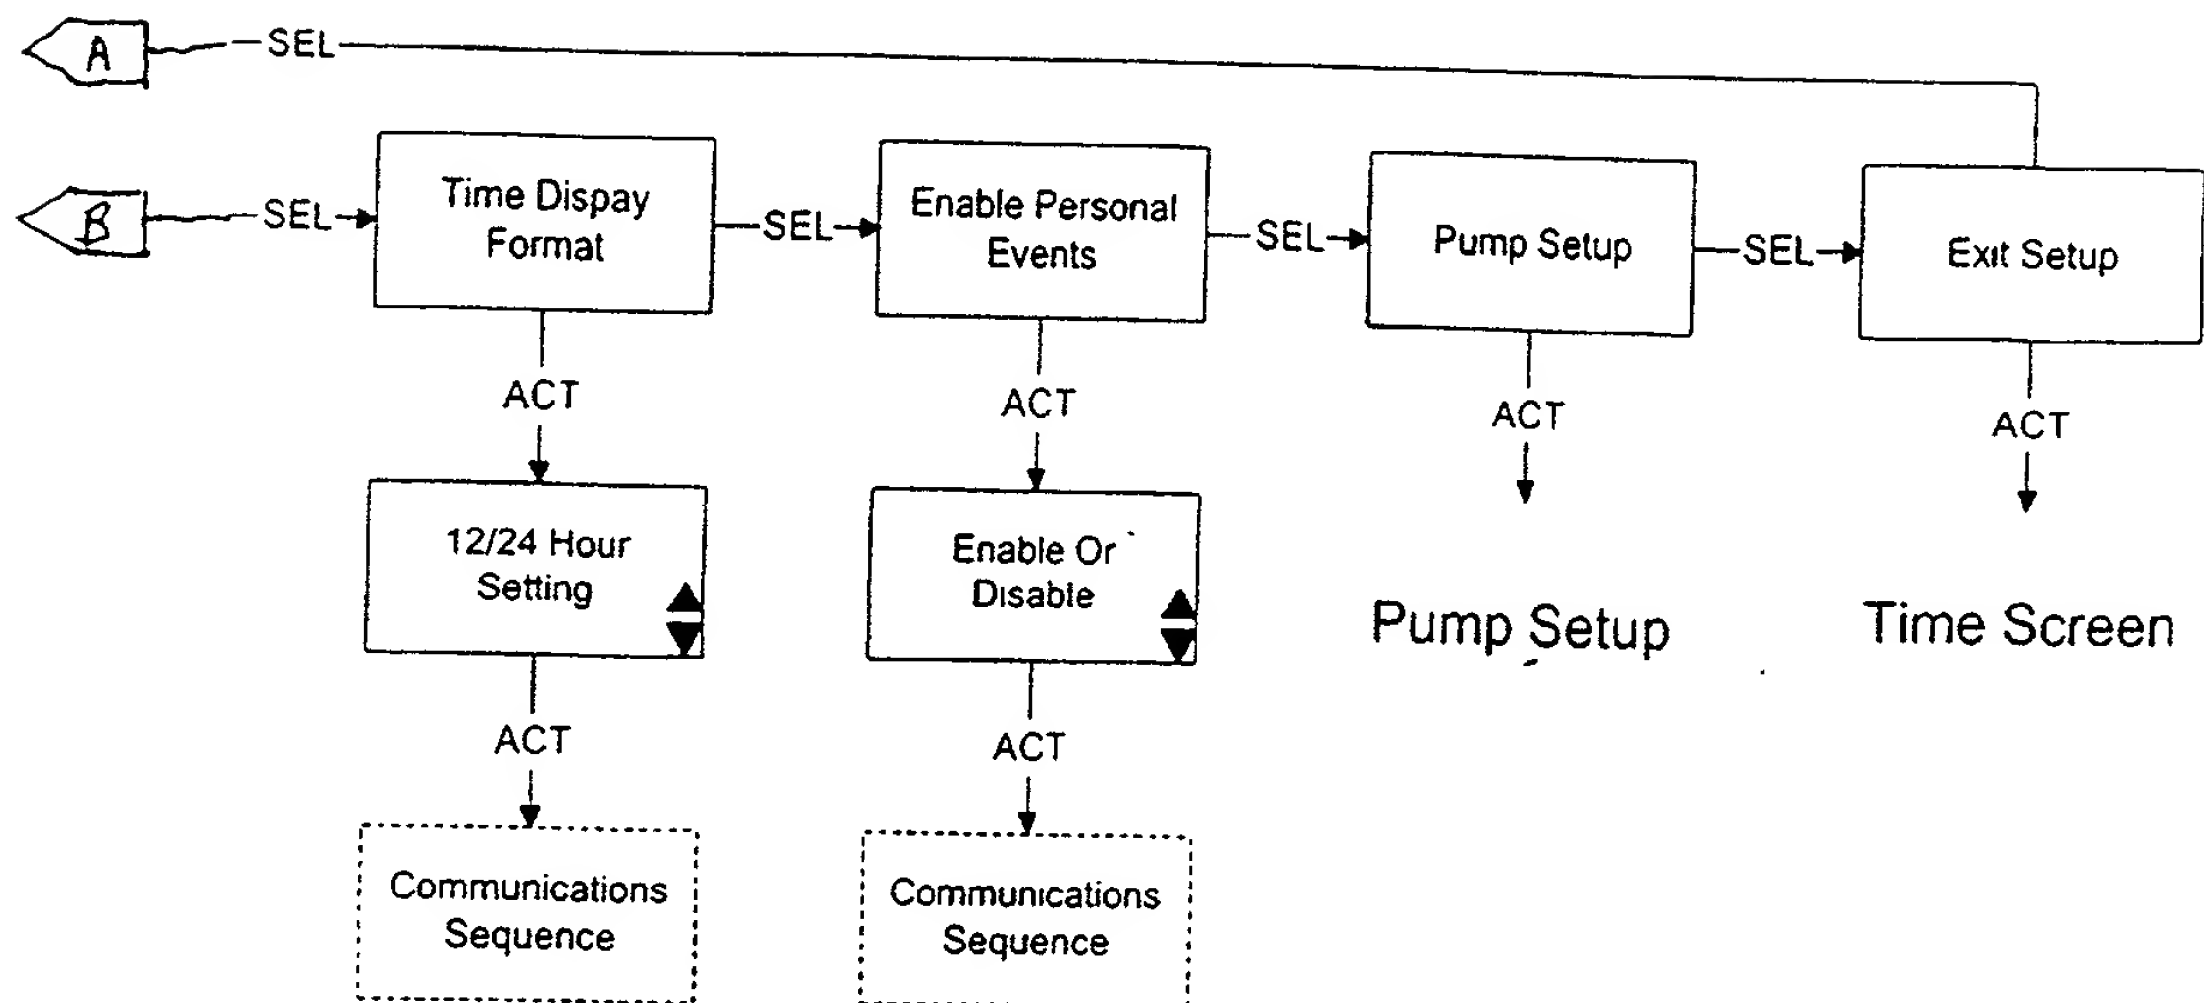


FIGURE 9b

Supervisor Menu

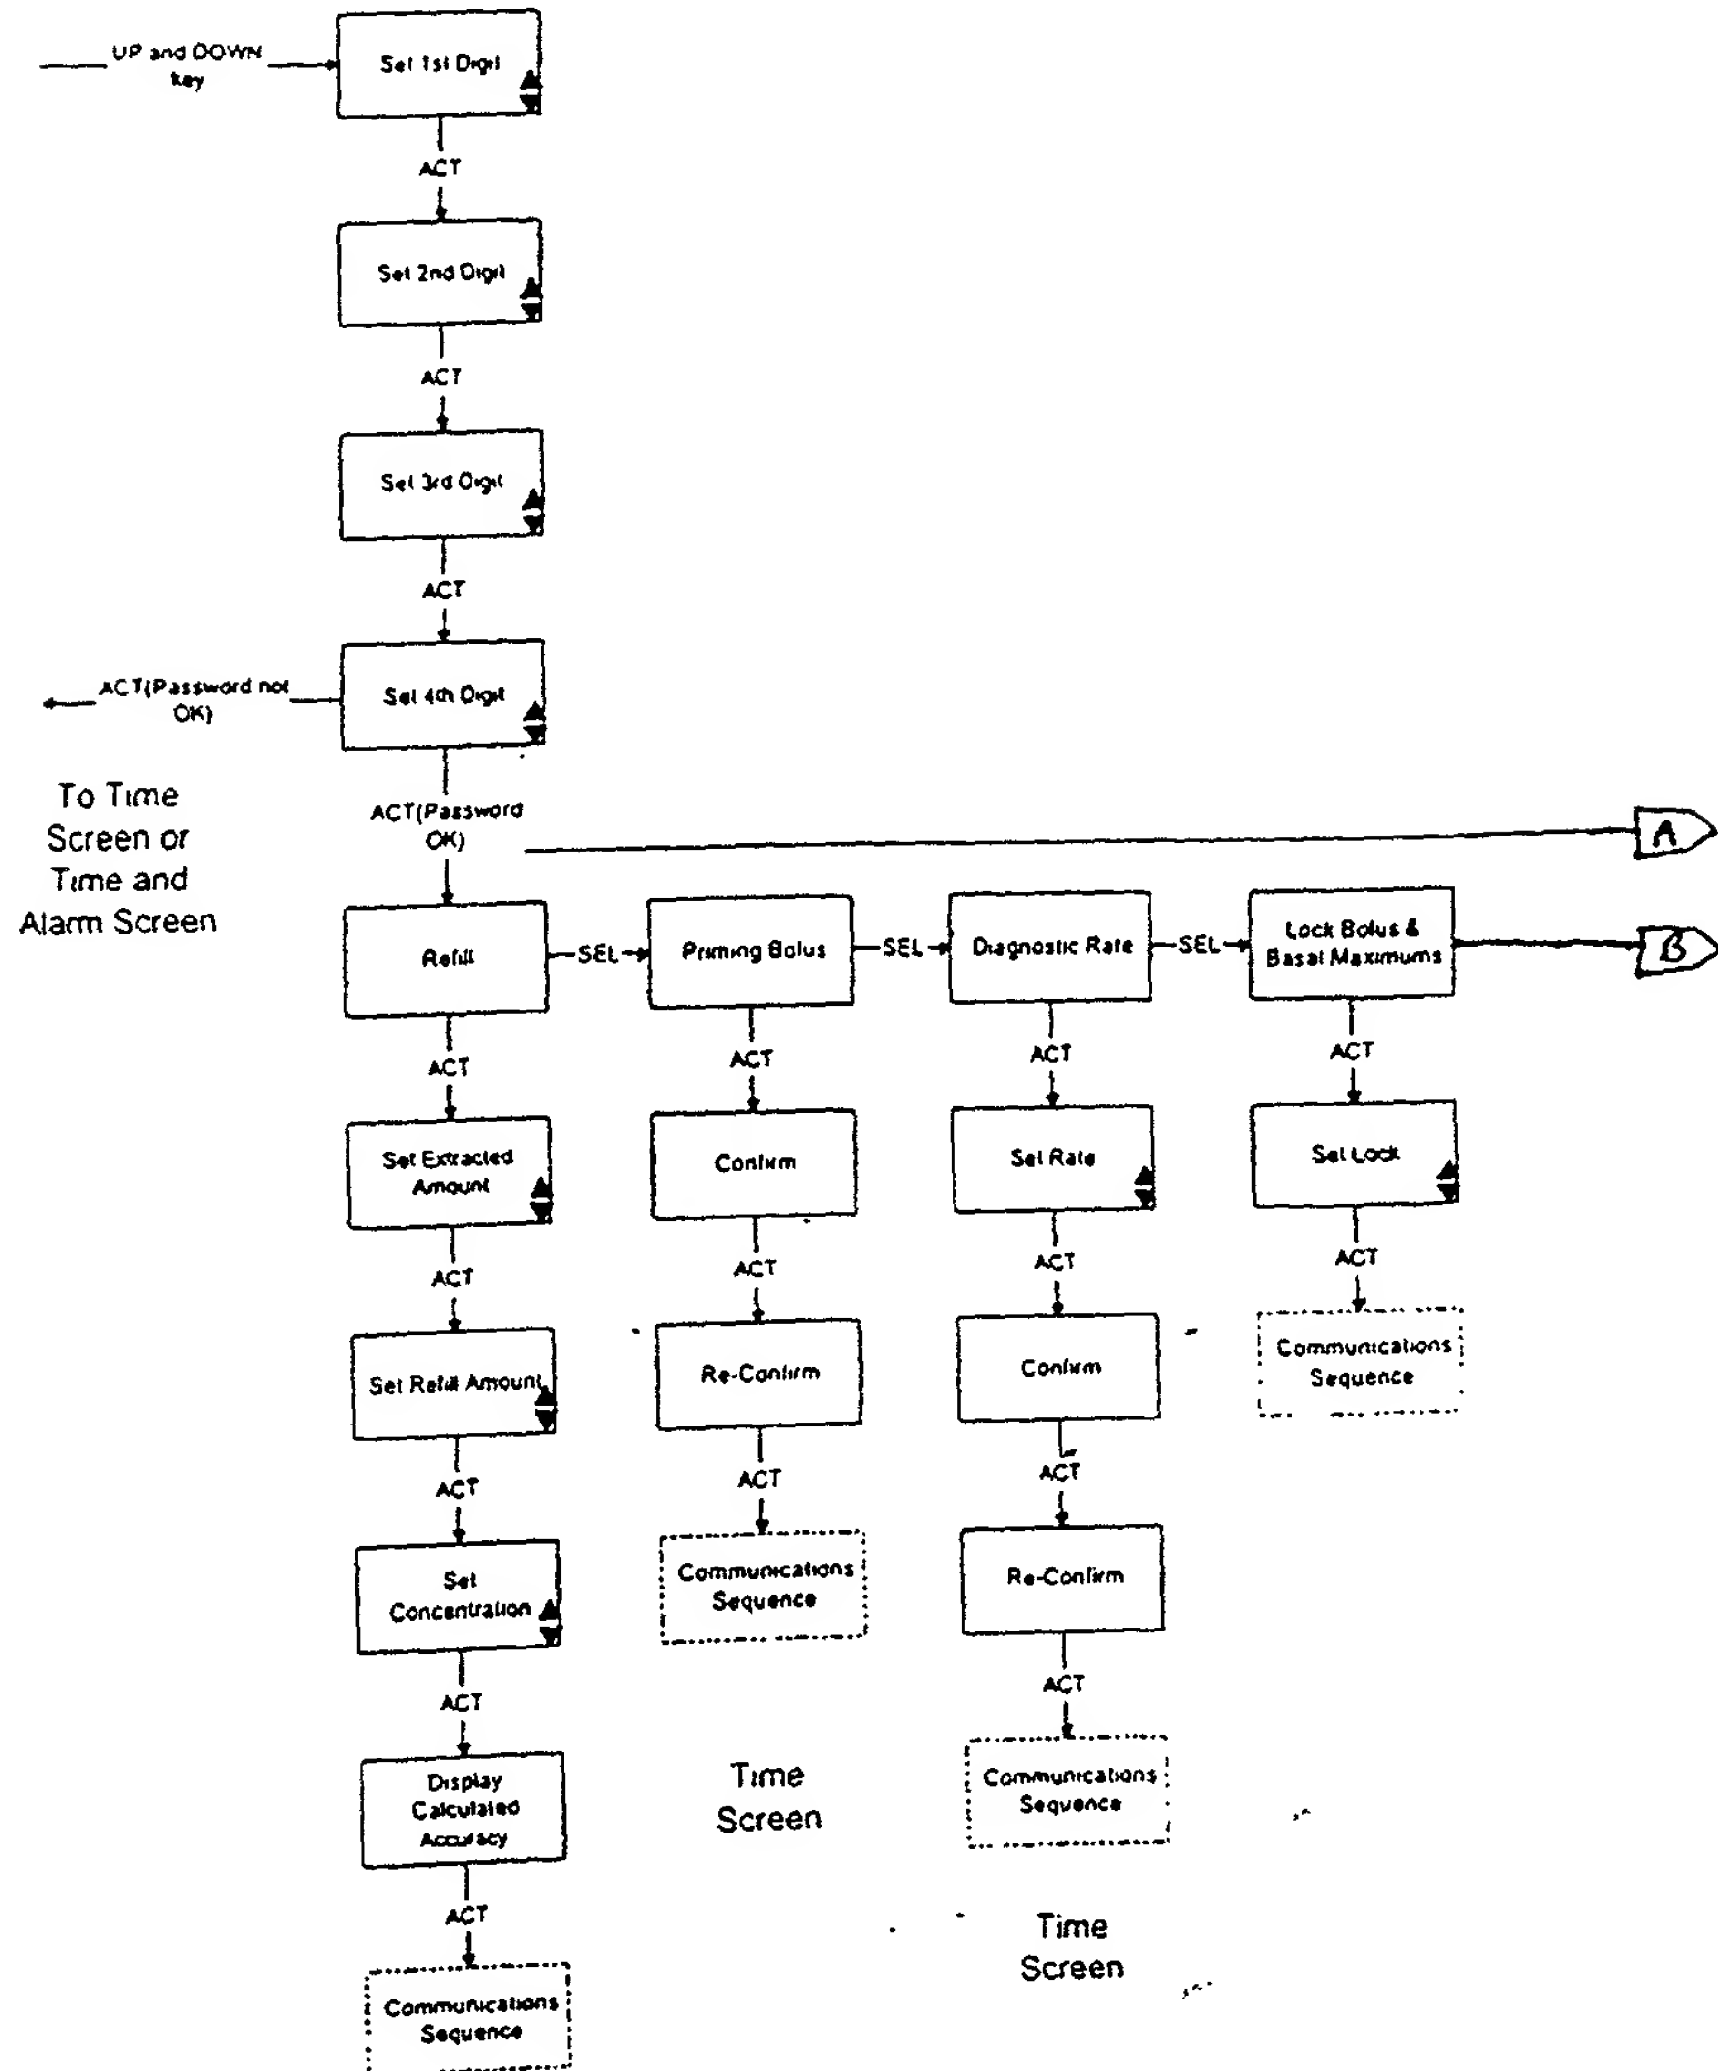

Unless otherwise shown, the screen that follows the Communications Sequence, shall be the next screen on the menu

FIGURE 10a

AMBULATORY MEDICAL APPARATUS WITH
HAND HELD COMMUNICATION DEVICE

Attorney: Ted Rittmaster - 047711-0221

Foley & Lardner - 310-277-2223

Sheet 15 of 16

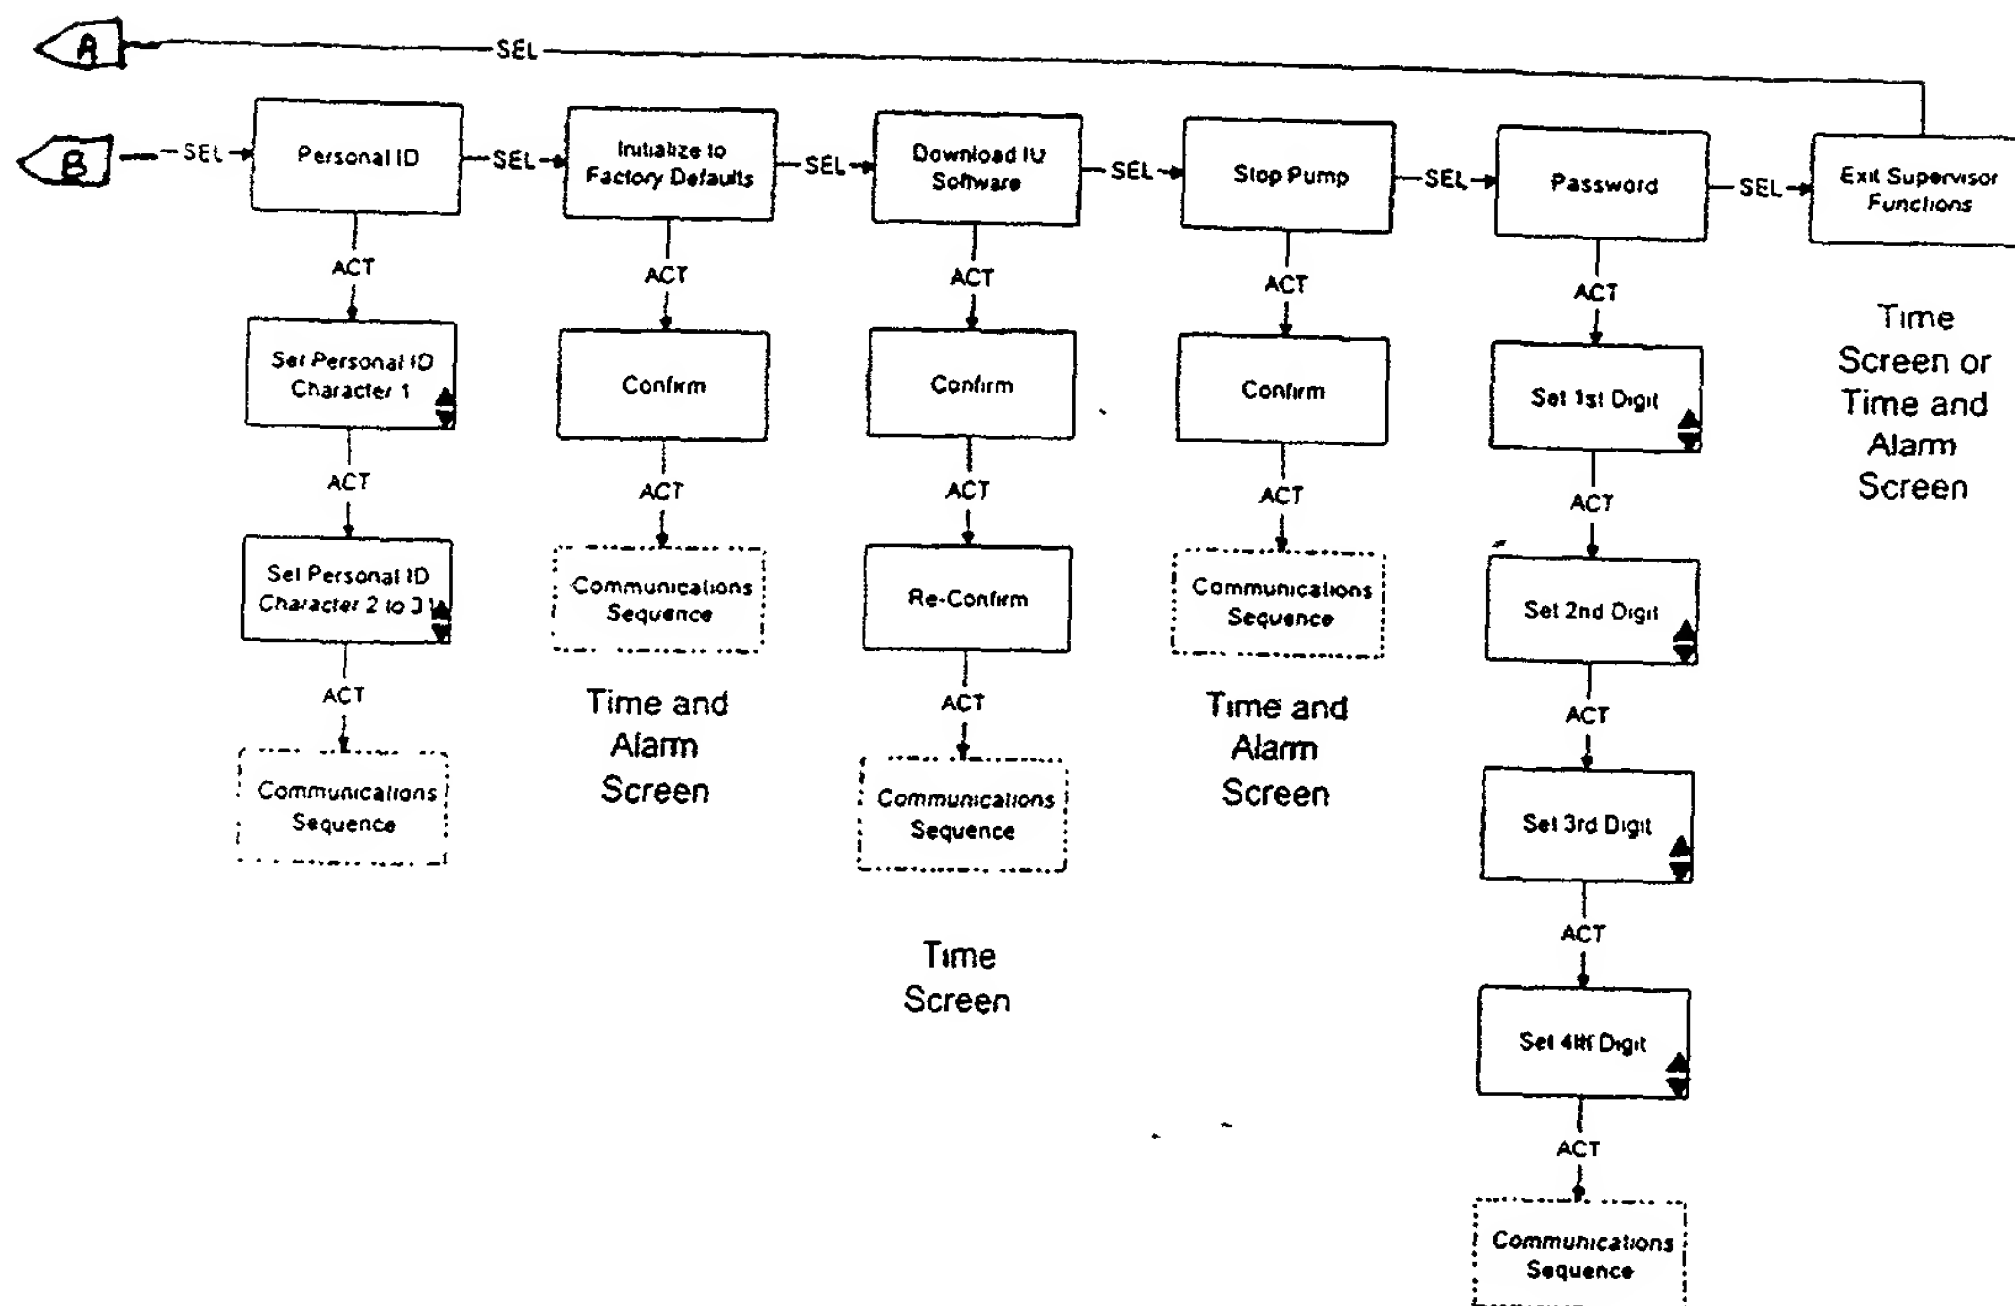


FIGURE 10b

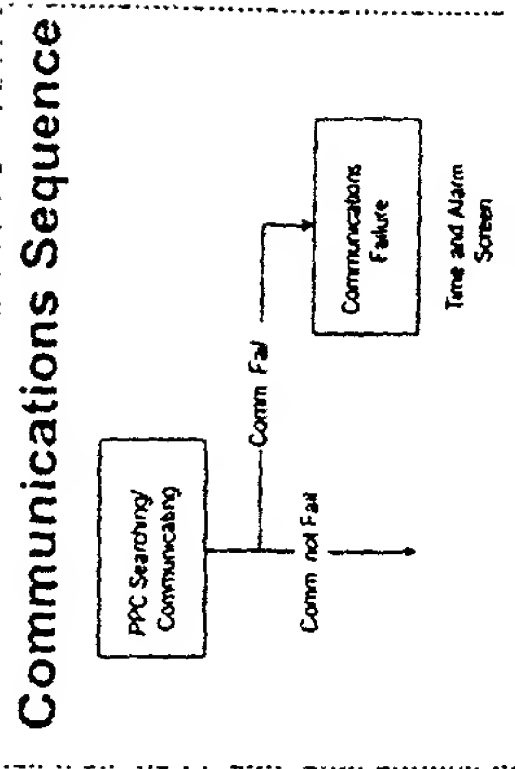


FIGURE 12

Sequences

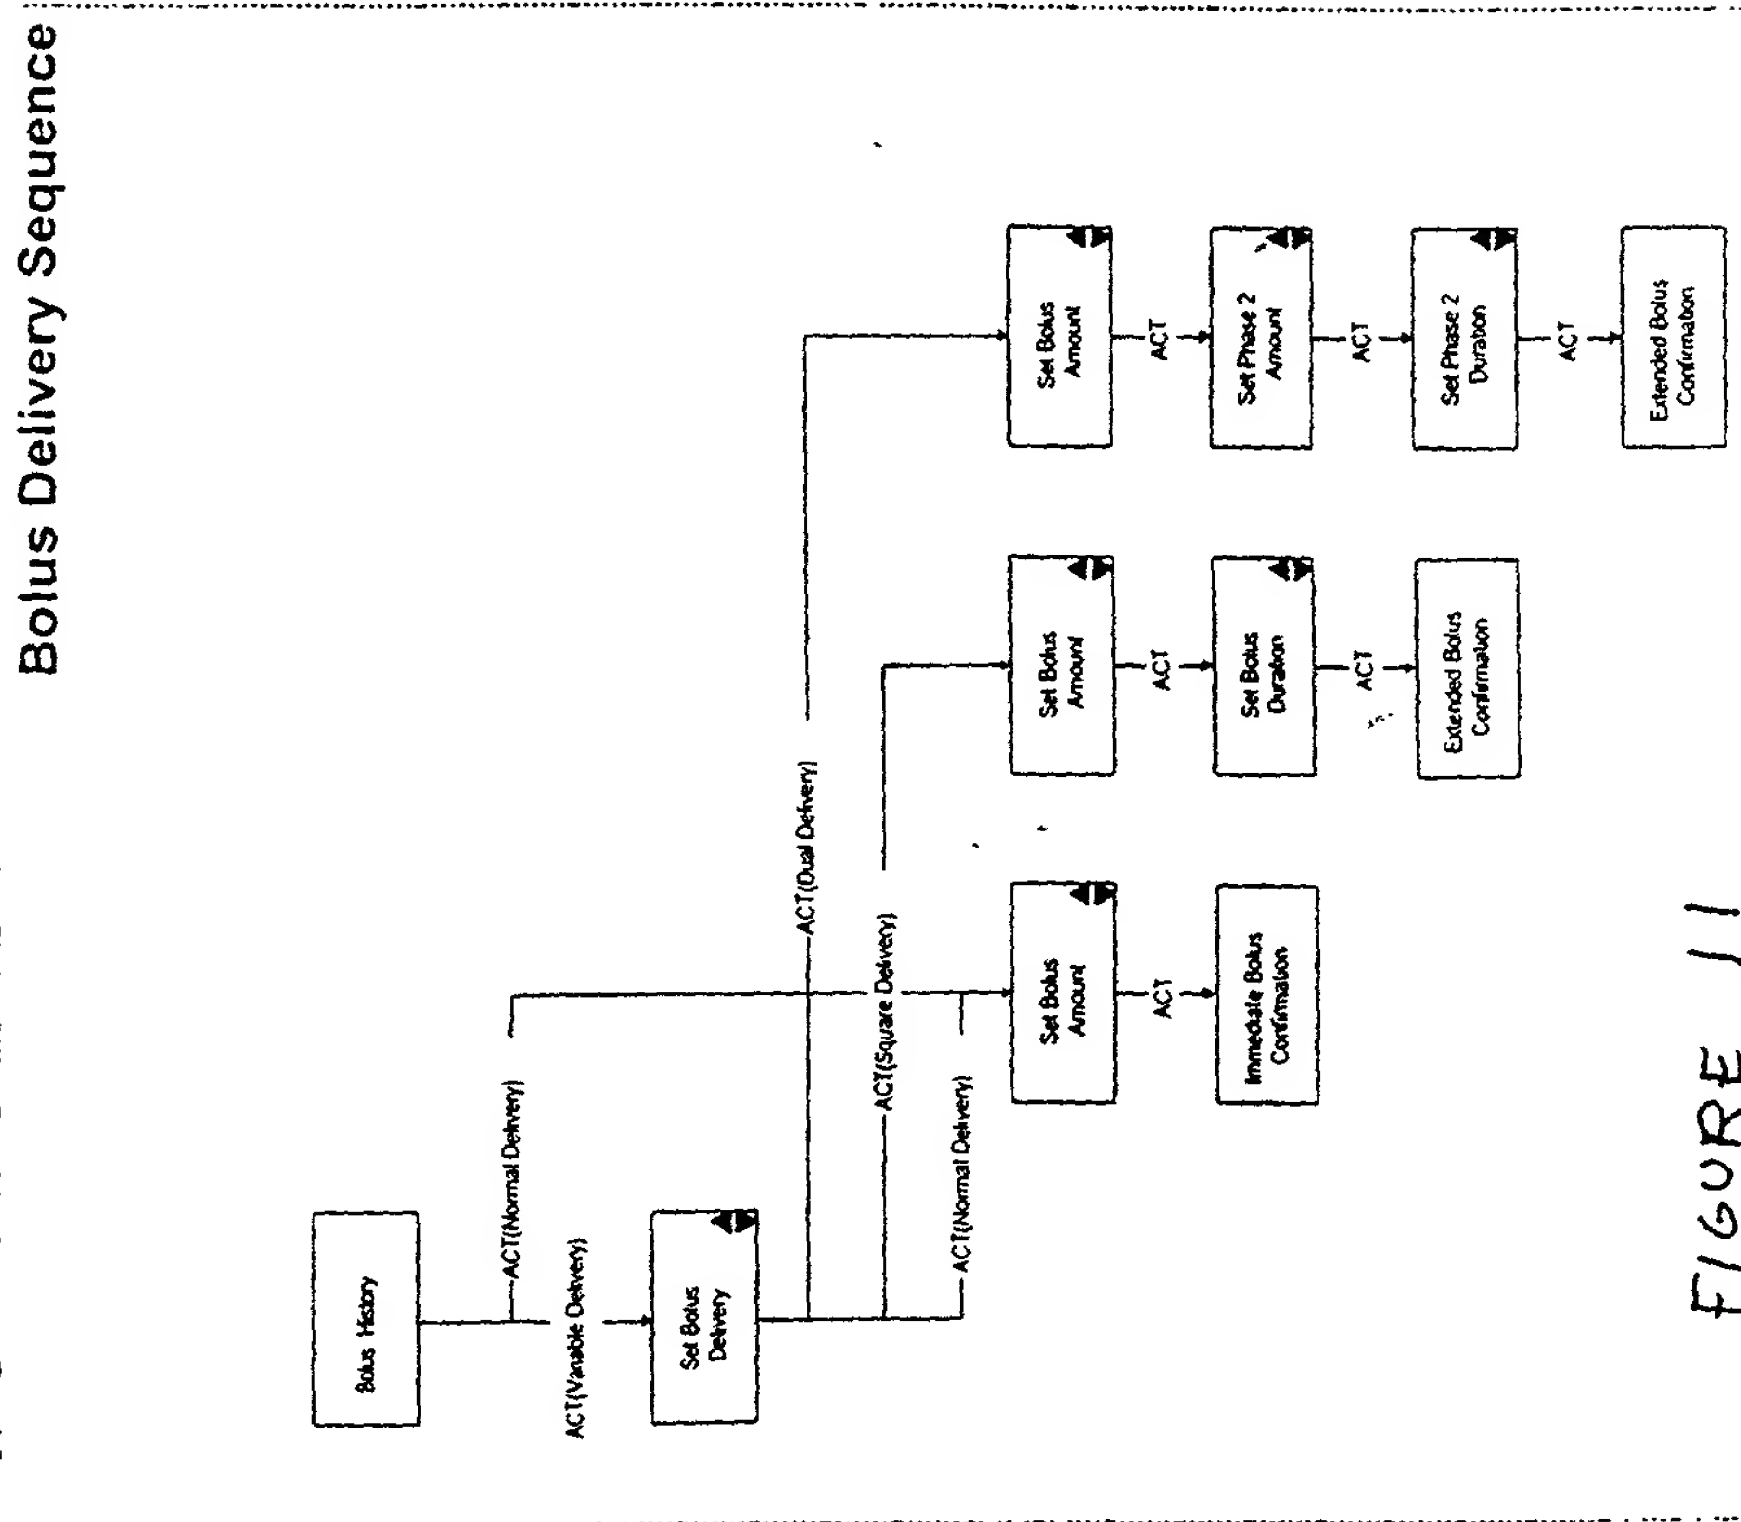


FIGURE 11